




2,5-Dimethylmethcathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



EI Mass Spectrum, 2,5-DMMC HCl Lot N17-P95D

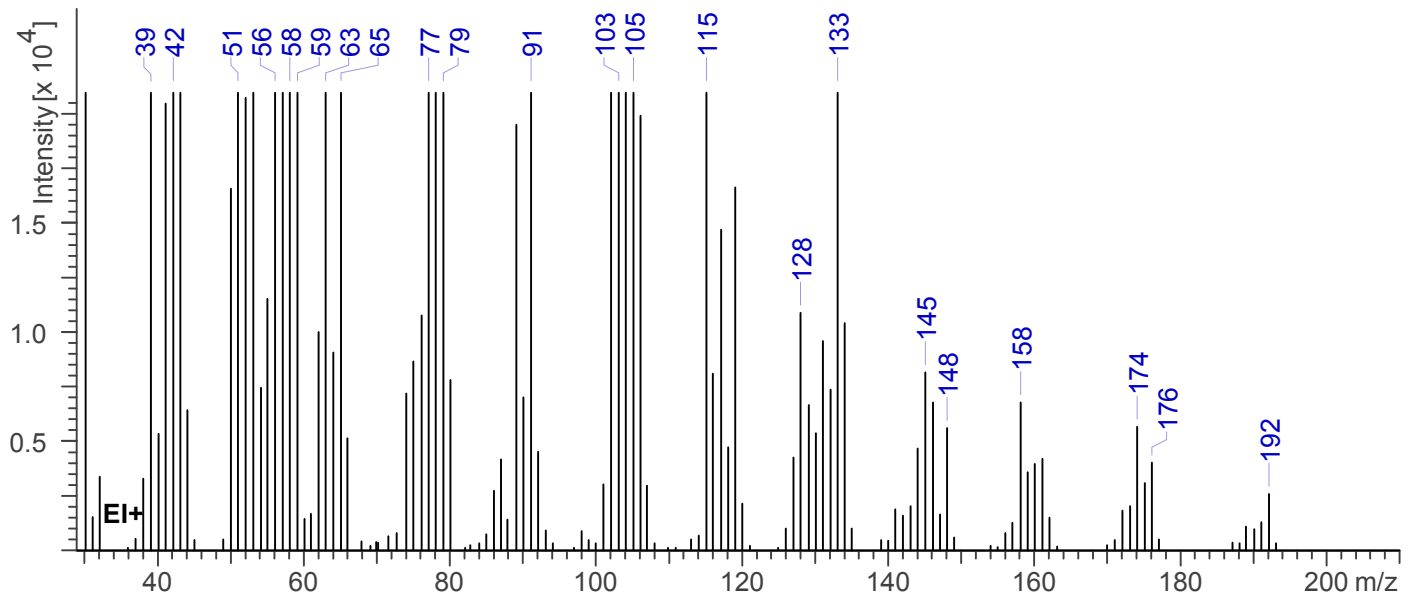


3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR with diamond ATR attachment (3 bounce)

Scan Parameters:
Number of scans: 32
Number of background scans: 32
Resolution: 4 cm⁻¹
Sample gain: 8
Aperture: 150

FTIR, ATR (Diamond, 3 Bounce) 2,5-DMMC HCl Lot N17-P95D

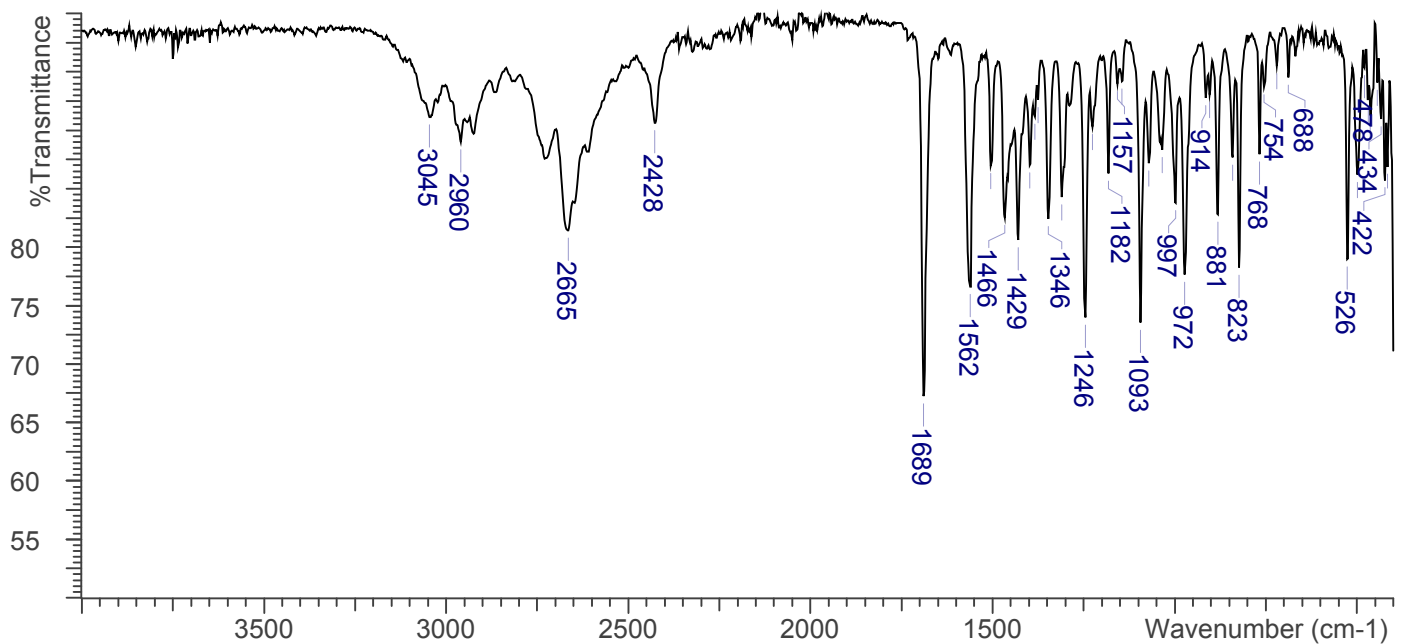




2,5-Dimethylmethcathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



FTIR, ATR (Diamond, 3 Bounce) 2,5-DMMC HCl Lot N17-P95D

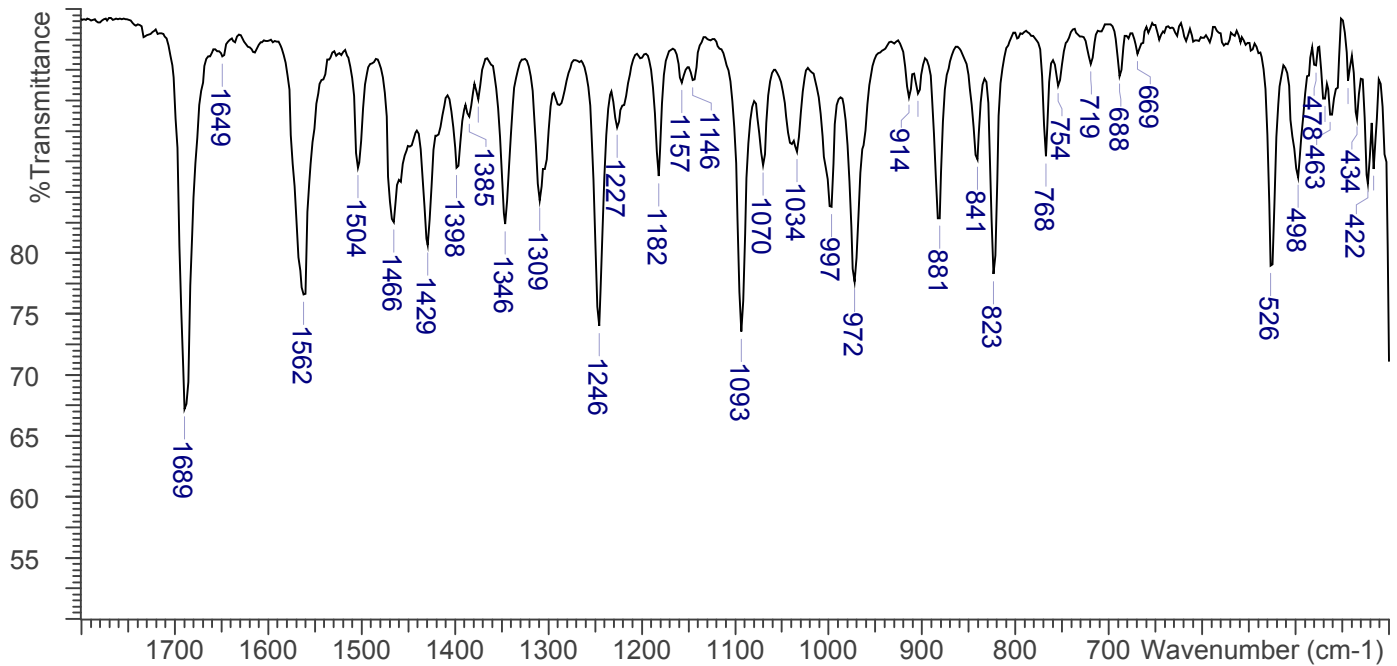

4. ADDITIONAL RESOURCES

No additional references as of 12/2013