




## 2-Fluoroisocathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

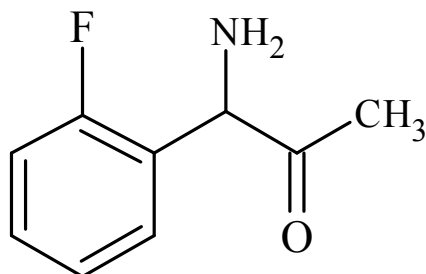

### 1. GENERAL INFORMATION

**IUPAC Name:** 1-amino-1-(2-fluorophenyl)propan-2-one

**CFR:** Not Scheduled (11/2013)

**CAS#:** Not Available

**Synonyms:** 2-FIC

**Source:** DEA Reference Material Collection

**Appearance:** White powder (HCl)

**UV<sub>max</sub> (nm):** Not Determined

### 2. CHEMICAL AND PHYSICAL DATA

#### 2.1 CHEMICAL DATA

Form	Chemical Formula	Molecular Weight	Melting Point (°C)
Base	C <sub>9</sub> H <sub>10</sub> FNO	167	Not Determined
HCl	C <sub>9</sub> H <sub>10</sub> FNO · HCl	203	195.0



## 2-Fluoroisocathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




### 3. QUALITATIVE DATA

#### 3.1 NUCLEAR MAGNETIC RESONANCE

**Sample Preparation:** Dilute analyte to ~5 mg/mL in deuterium oxide (D<sub>2</sub>O) containing TSP for 0 ppm reference and maleic acid as quantitative internal standard.

**Instrument:** 400 MHz NMR spectrometer  
**Parameters:** Spectral width: at least containing -3 ppm through 13 ppm  
Pulse angle: 90°  
Delay between pulses: 45 seconds

<sup>1</sup>H NMR: 2-Fluoroisocathinone HCl; Lot 0450088-3; D<sub>2</sub>O; 400MHz

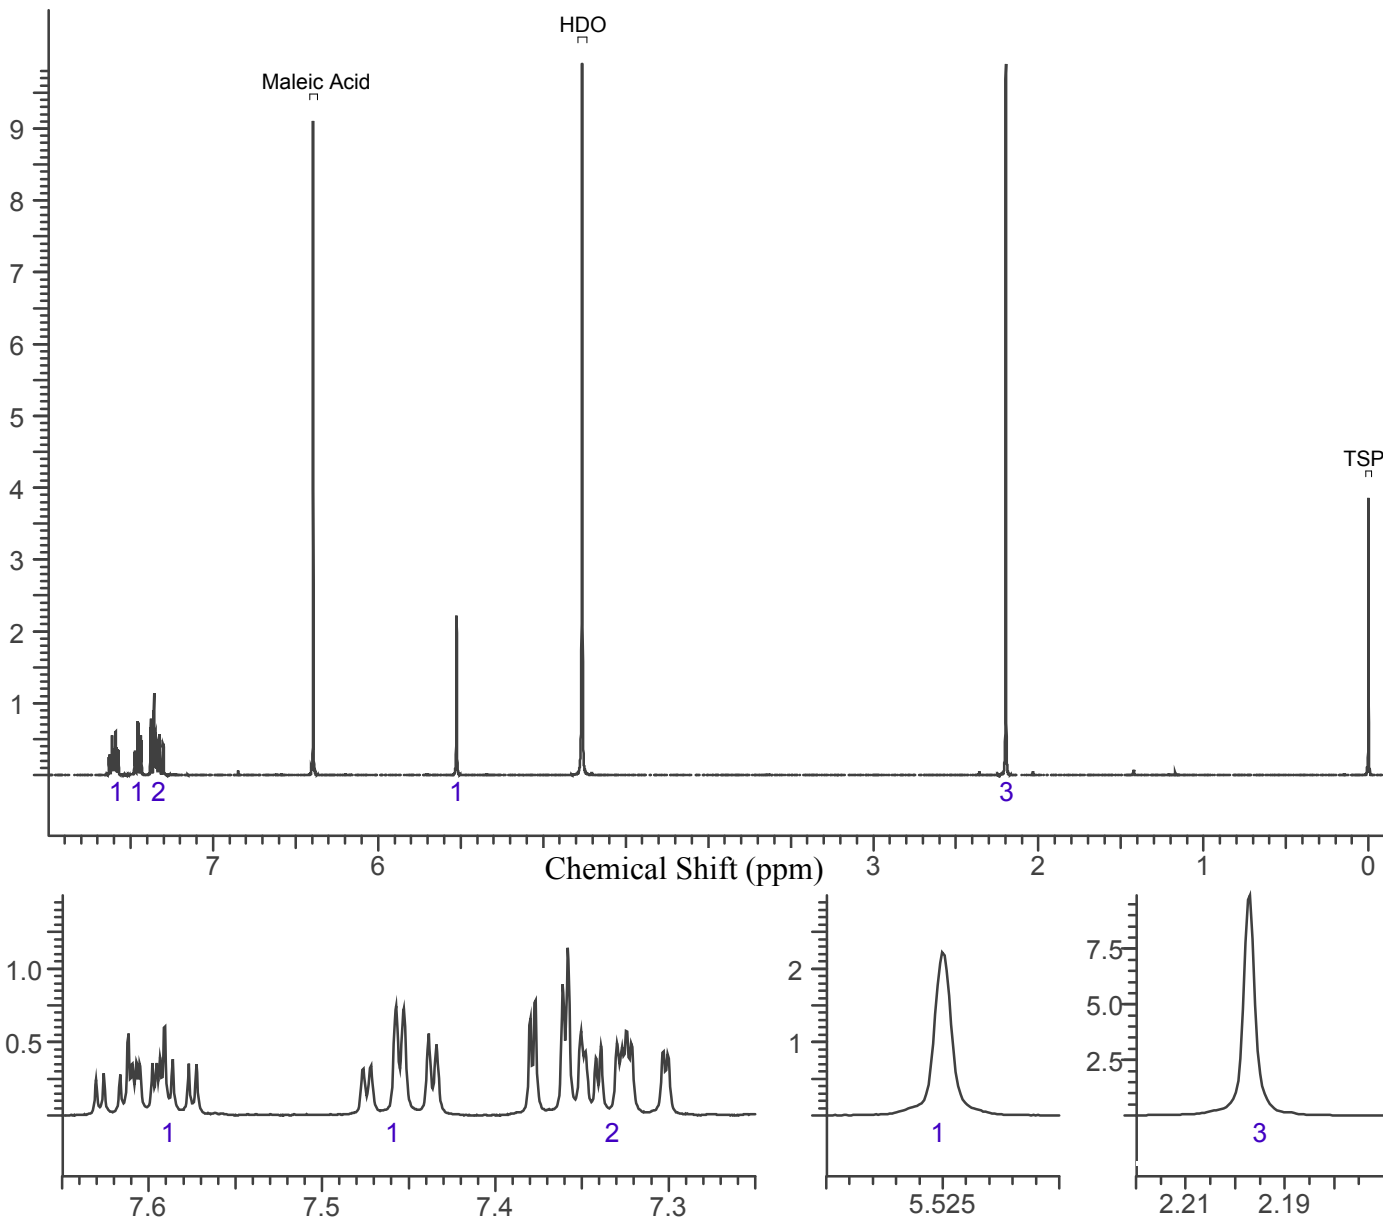



## 2-Fluoroisocathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



### 3.2 Gas Chromatography/Mass Spectrometry

**Sample Preparation:** Dilute analyte ~ 5 mg/mL base extracted into chloroform

**Instrument:** Agilent gas chromatograph operated in split mode with MS detector

**Column:** DB-1 MS (or equivalent); 30m x 0.25 mm x 0.25  $\mu$ m

**Carrier Gas:** Helium at 1 mL/min

**Temperatures:** Injector: 280°C  
MSD transfer line: 280°C

MS Source: 230°C

MS Quad: 150°C

Oven program:

1) 100°C initial temperature for 1.0 min

2) Ramp to 300°C at 12 °C/min

3) Hold final temperature for 9.0 min

**Injection Parameters:** Split Ratio = 20:1, 1  $\mu$ L injected

**MS Parameters:** Mass scan range: 30-550 amu


Threshold: 100

Tune file: stune.u

Acquisition mode: scan

**Retention Time:** 5.311 min

EI Mass Spectrum: 2-Fluoroisocathinone HCl; Lot 0450088-3

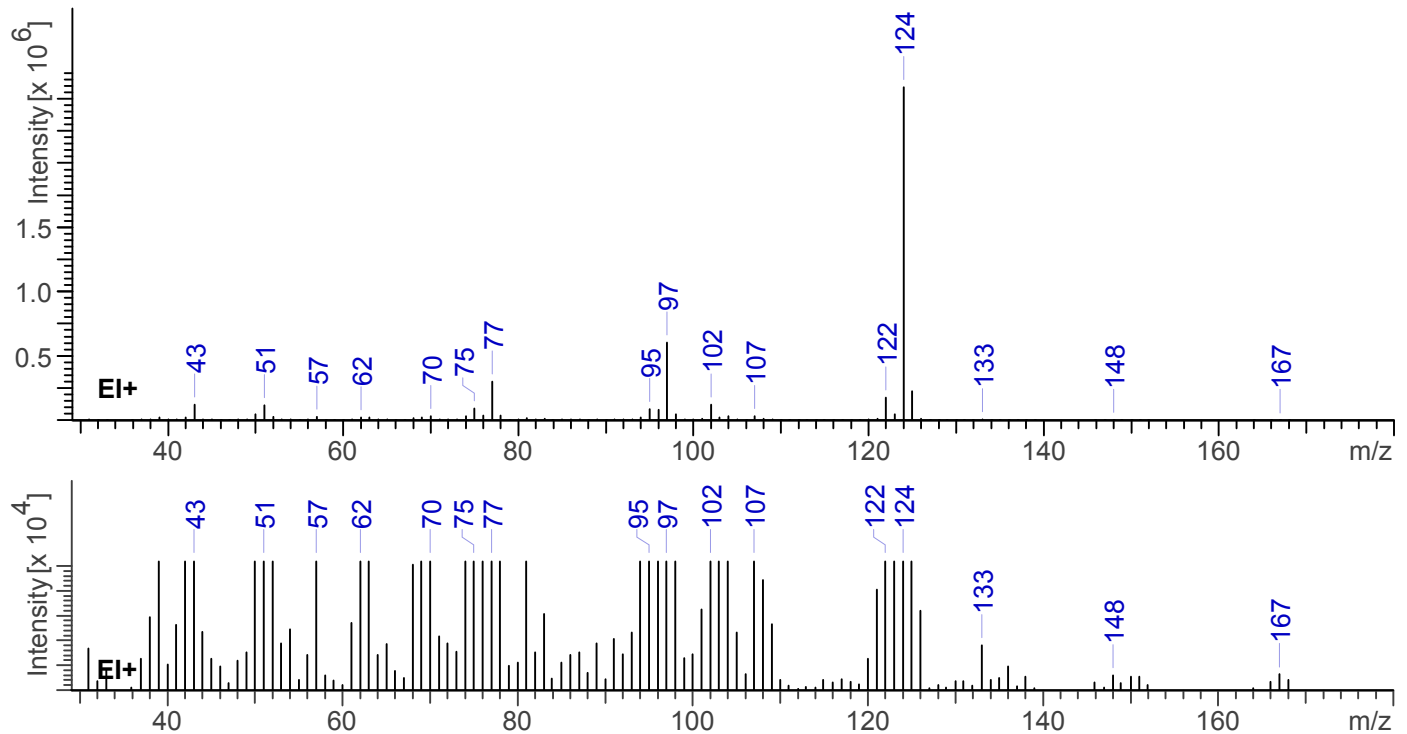



## 2-Fluoroisocathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.





### 3.3 INFRARED SPECTROSCOPY (FTIR)

**Instrument:** FTIR with diamond ATR attachment (3 bounce)

**Scan Parameters:**  
Number of scans: 32  
Number of background scans: 32  
Resolution: 4 cm<sup>-1</sup>  
Sample gain: 8  
Aperture: 150

FTIR ATR (Diamond, 3 bounce): 2-Fluoroisocathinone HCl; Lot 0450088-3

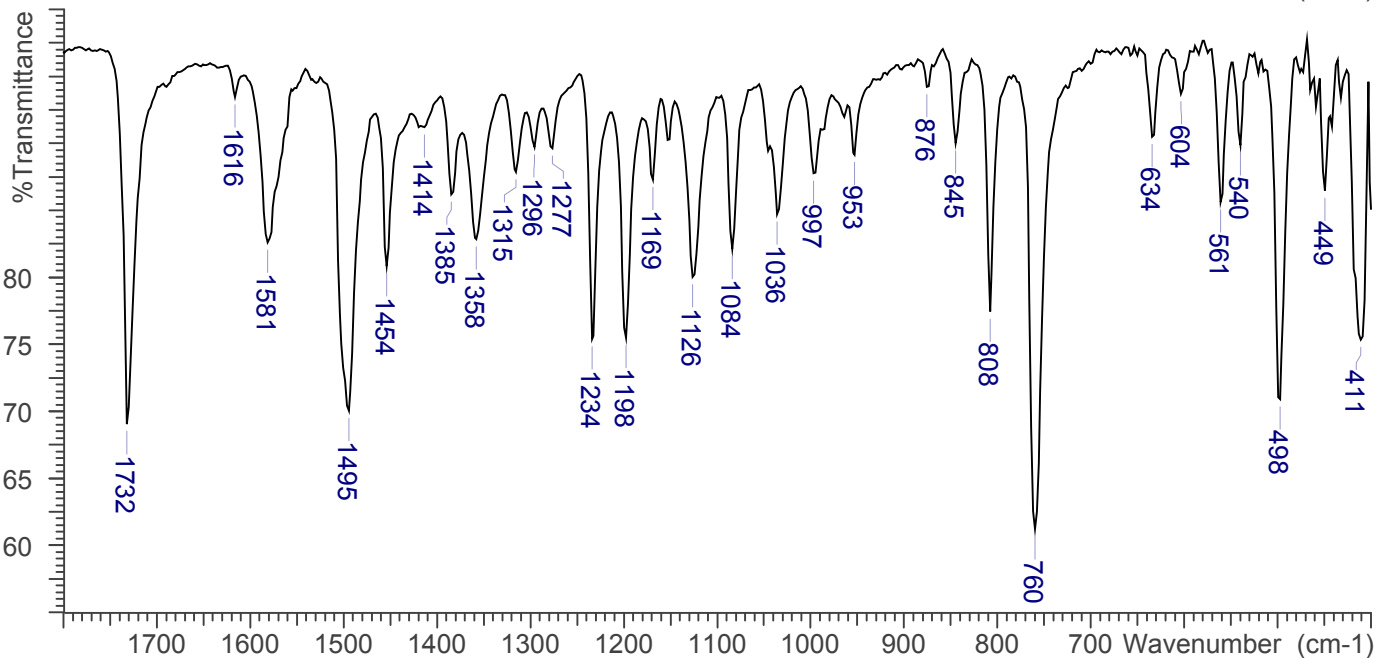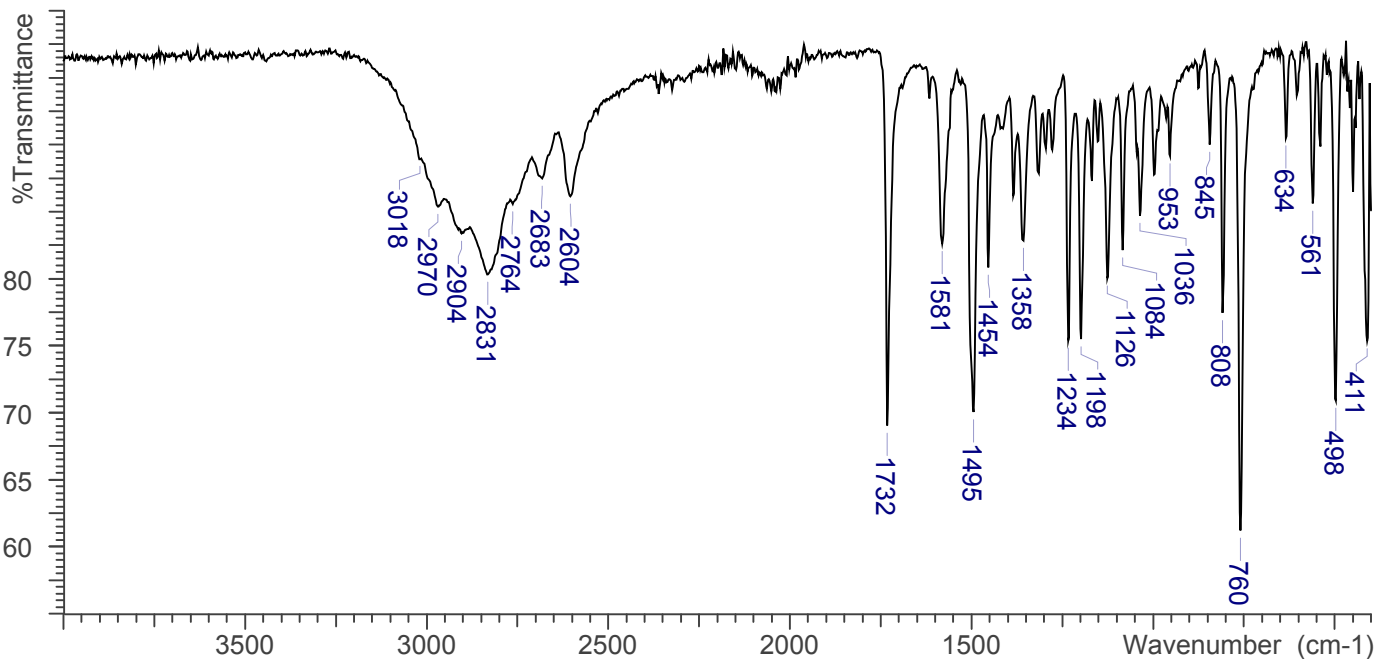



## 2-Fluoroisocathinone

*The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.*



### 4. **ADDITIONAL RESOURCES**

No resources identified as of 11/2013.