




25C-NB4OMe

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

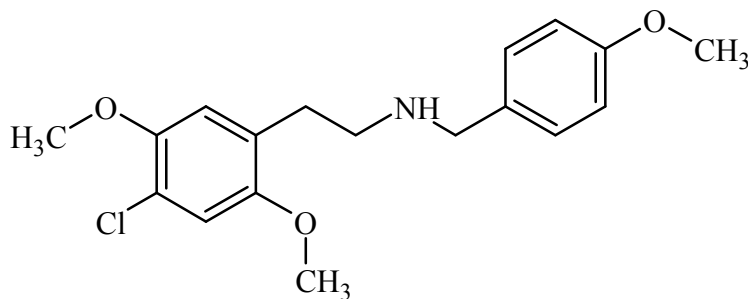

1. GENERAL INFORMATION

IUPAC Name: 2-(4-chloro-2,5-dimethoxyphenyl)-N-(4-methoxybenzyl)ethanamine

CAS#: Not Available

Synonyms: N-(4-methoxybenzyl)-2-(4-chloro-2,5-dimethoxyphenyl)ethylamine
4-Methoxy-25C-NBOMe

Source: DEA Reference Material Collection

Appearance: White powder

UV_{max}(nm): Not Determined

2. CHEMICAL AND PHYSICAL DATA

2.1 CHEMICAL DATA

Form	Chemical Formula	Molecular Weight	Melting Point (°C)
Base	C ₁₈ H ₂₂ ClNO ₃	335	Not Determined
HCl	C ₁₈ H ₂₂ ClNO ₃ HCl	372	189.1



25C-NB4OMe

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




3. QUALITATIVE DATA

3.1 NUCLEAR MAGNETIC RESONANCE

Sample Preparation: Dilute analyte to ~10 mg/mL in CDCl₃ containing TMS for 0 ppm reference and methenamine as quantitative internal standard.

Instrument: 400 MHz NMR spectrometer
Parameters: Spectral width: at least containing -3 ppm through 13 ppm
Pulse angle: 90°
Delay between pulses: 45 seconds

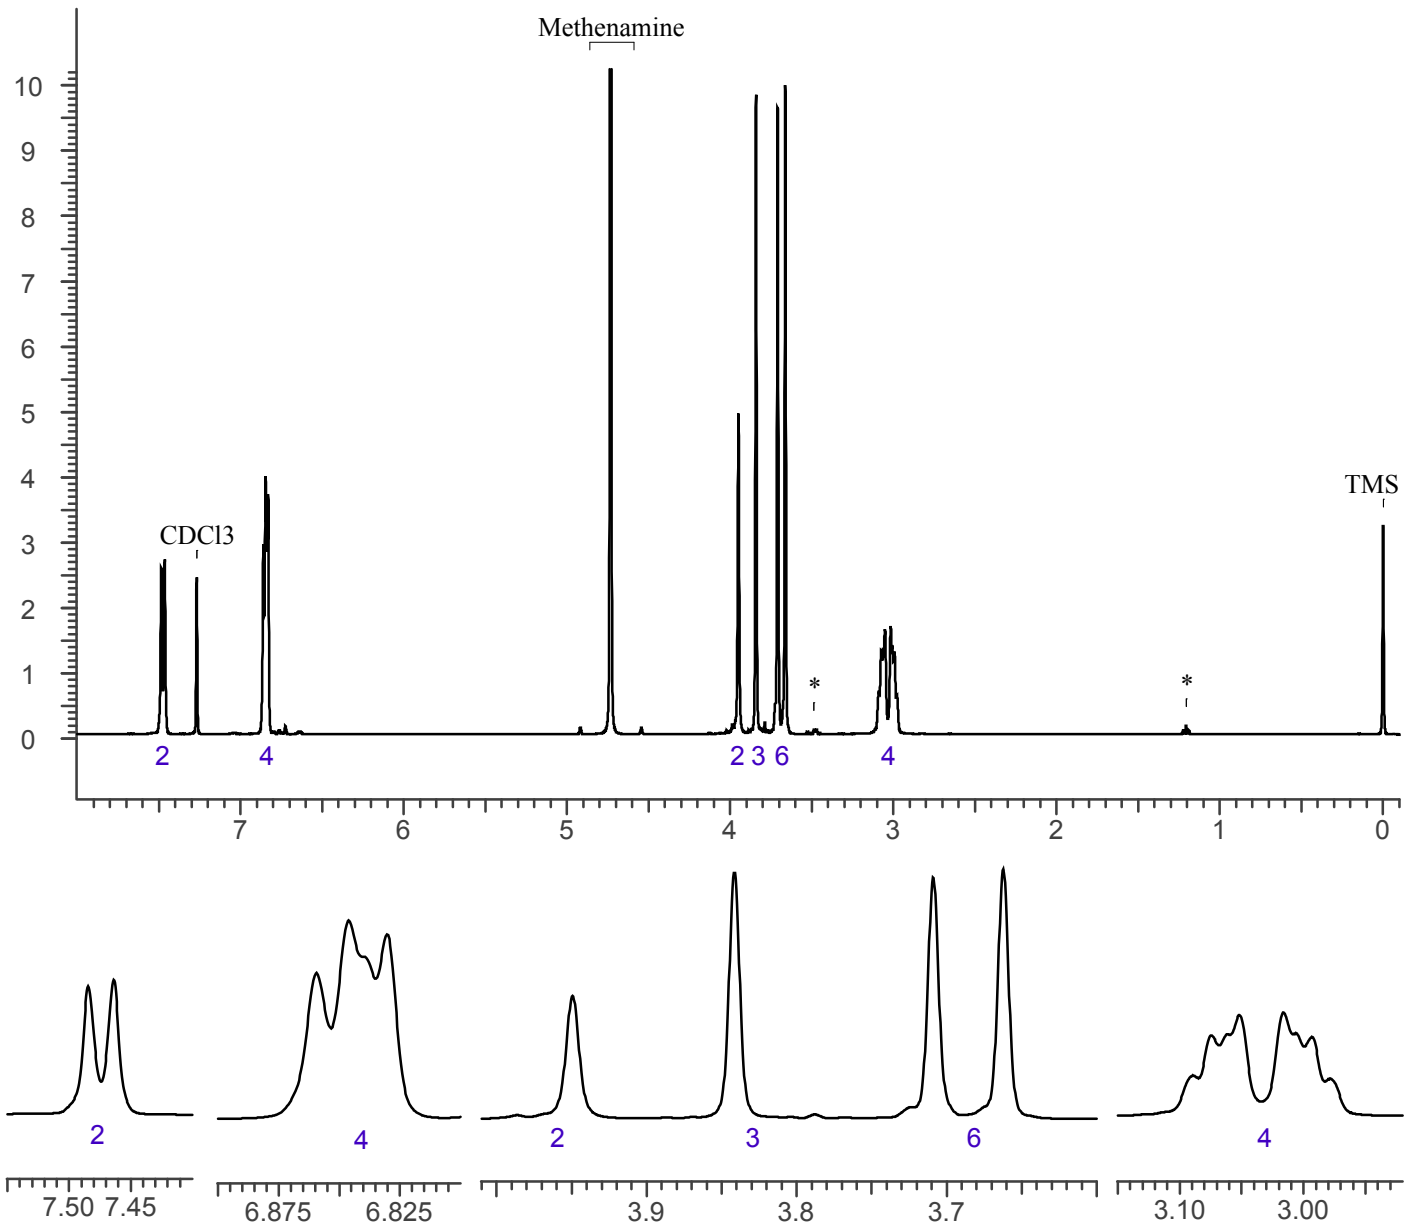



25C-NB4OMe

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




3.2 GAS CHROMATOGRAPHY/MASS SPECTROMETRY

Sample Preparation: Dilute analyte ~4 mg/mL in CHCl₃.

Instrument: Agilent gas chromatograph operated in split mode with MS detector
Column: DB-1 MS (or equivalent); 30m x 0.25 mm x 0.25 μm
Carrier Gas: Helium at 1 mL/min
Temperatures: Injector: 280°C
MSD transfer line: 280°C
MS Source: 230°C
MS Quad: 150°C
Oven program:
1) 100°C initial temperature for 1.0 min
2) Ramp to 300°C at 12 °C/min
3) Hold final temperature for 9.0 min

Injection Parameters: Split Ratio = 20:1, 1 μL injected
MS Parameters: Mass scan range: 30-550 amu
Threshold: 100
Tune file: stune.u
Acquisition mode: scan
Retention Time: 15.534 min

EI Mass Spectrum 25C-NB4OMe HCl Lot N17-P73C

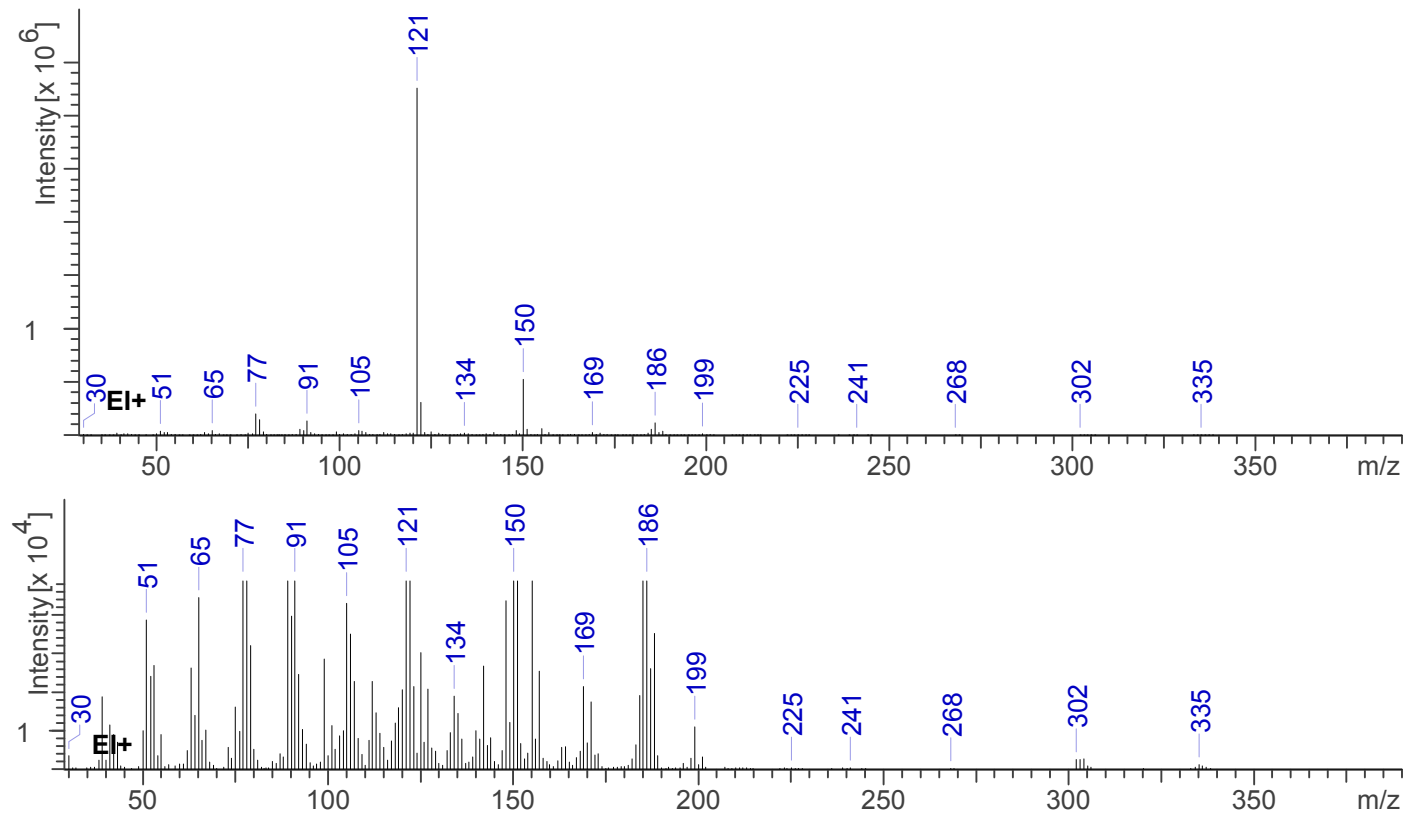



25C-NB4OMe

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR with diamond ATR attachment (3 bounce)

Scan Parameters:
Number of scans: 32
Number of background scans: 32
Resolution: 4 cm^{-1}
Sample gain: 8
Aperture: 150

FTIR ATR (Diamond, 3 Bounce) 25C-NB4OMe HCl Lot N17-P73C

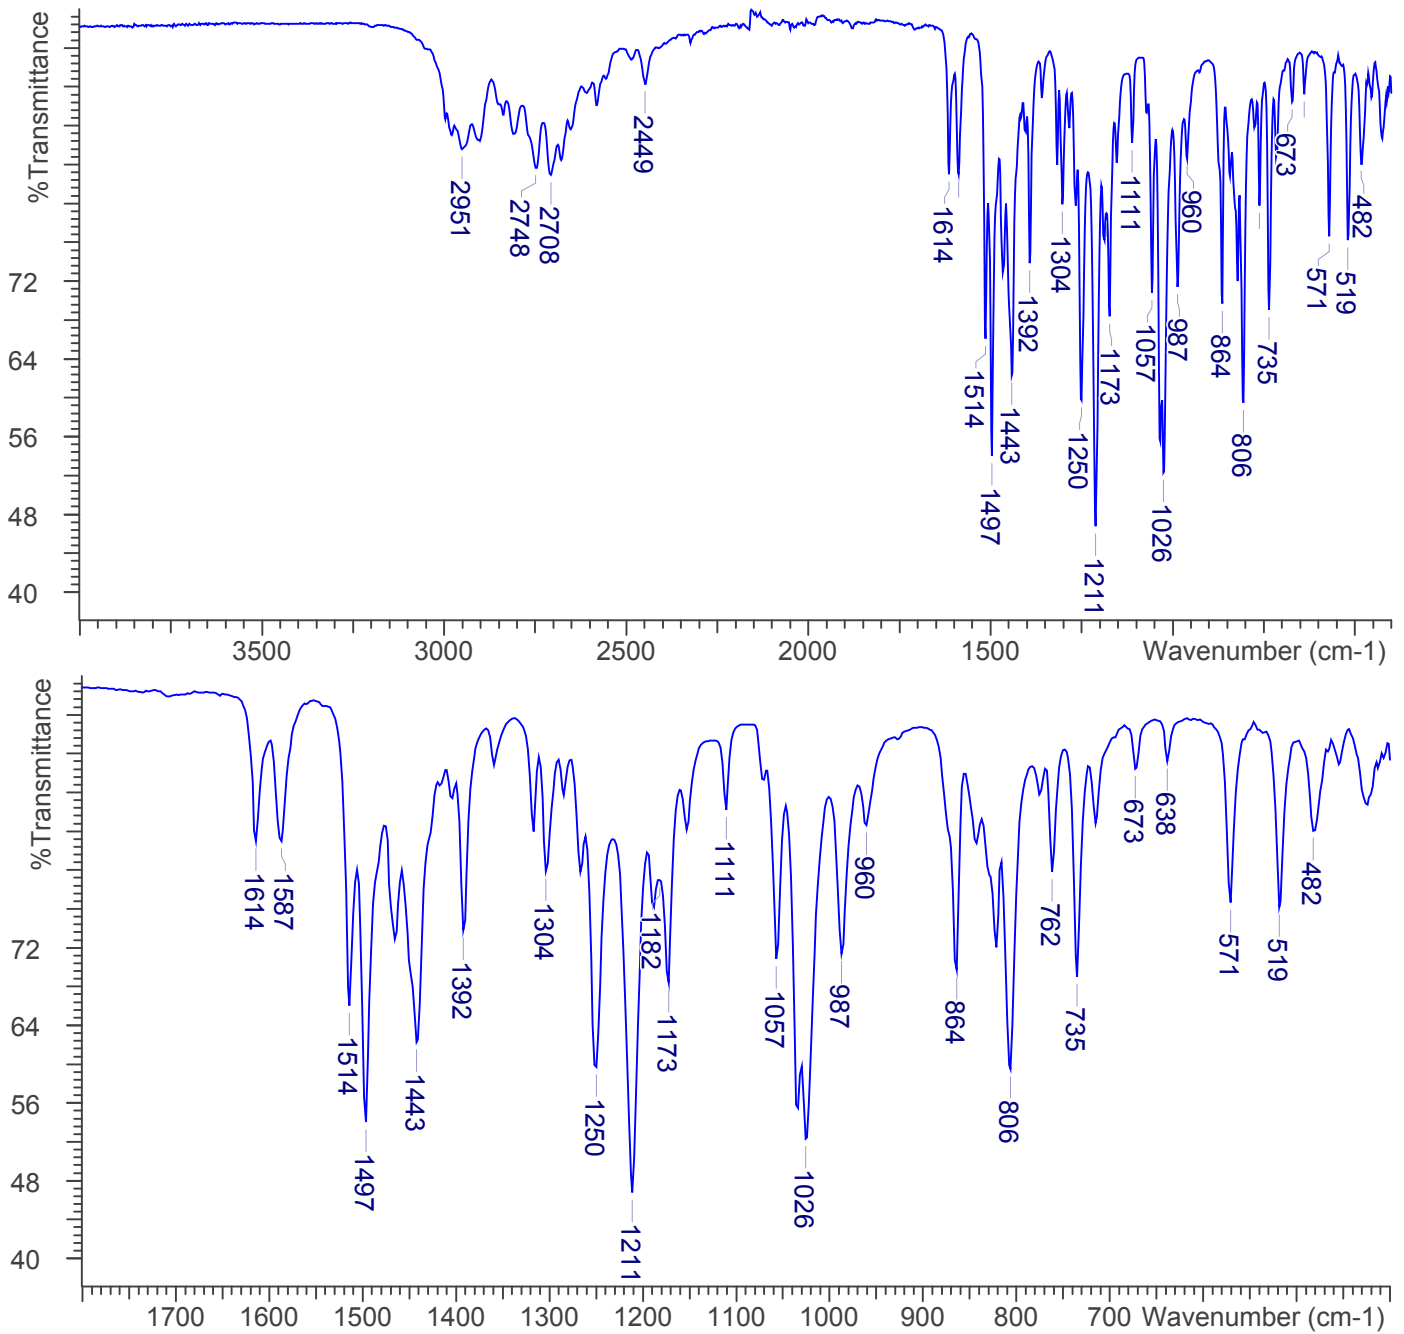



25C-NB4OMe

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



4. ADDITIONAL RESOURCES

<http://forendex.southernforensic.org/index.php/detail/index/1047>

ation from