




## 3,4-Methylenedioxy-N-benzylcathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

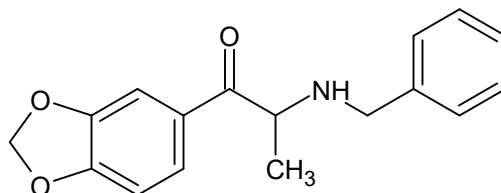

### 1. GENERAL INFORMATION

<b>IUPAC Name:</b>	1-(1,3-benzodioxol-5-yl)-2-(benzylamino)propan-1-one
<b>CAS#:</b>	1823274-68-5
<b>Synonyms:</b>	BMDP, 1-(2 <i>H</i> -1,3-benzodioxol-5-yl)-2-(benzylamino)propan-1-one
<b>Source:</b>	DEA Reference Material Collection
<b>Appearance:</b>	White powder
<b>UV<sub>max</sub>(nm):</b>	Not determined

### 2. CHEMICAL AND PHYSICAL DATA

#### 2.1 CHEMICAL DATA

Form	Chemical Formula	Molecular Weight	Melting Point (°C)
Base	C <sub>17</sub> H <sub>17</sub> NO <sub>3</sub>	283.32	Not Determined
HCl	C <sub>17</sub> H <sub>17</sub> NO <sub>3</sub> HCl	319.78	Not Determined



## 3,4-Methylenedioxy-N-benzylcathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




### 3. QUALITATIVE DATA

#### 3.1 NUCLEAR MAGNETIC RESONANCE

**Sample Preparation:** Dilute analyte to ~12 mg/mL in D<sub>2</sub>O containing TSP for 0 ppm reference and maleic acid as quantitative internal standard.

**Instrument:** 400 MHz NMR spectrometer  
**Parameters:** Spectral width: at least containing -3 ppm through 13 ppm  
Pulse angle: 90°  
Delay between pulses: 45 seconds

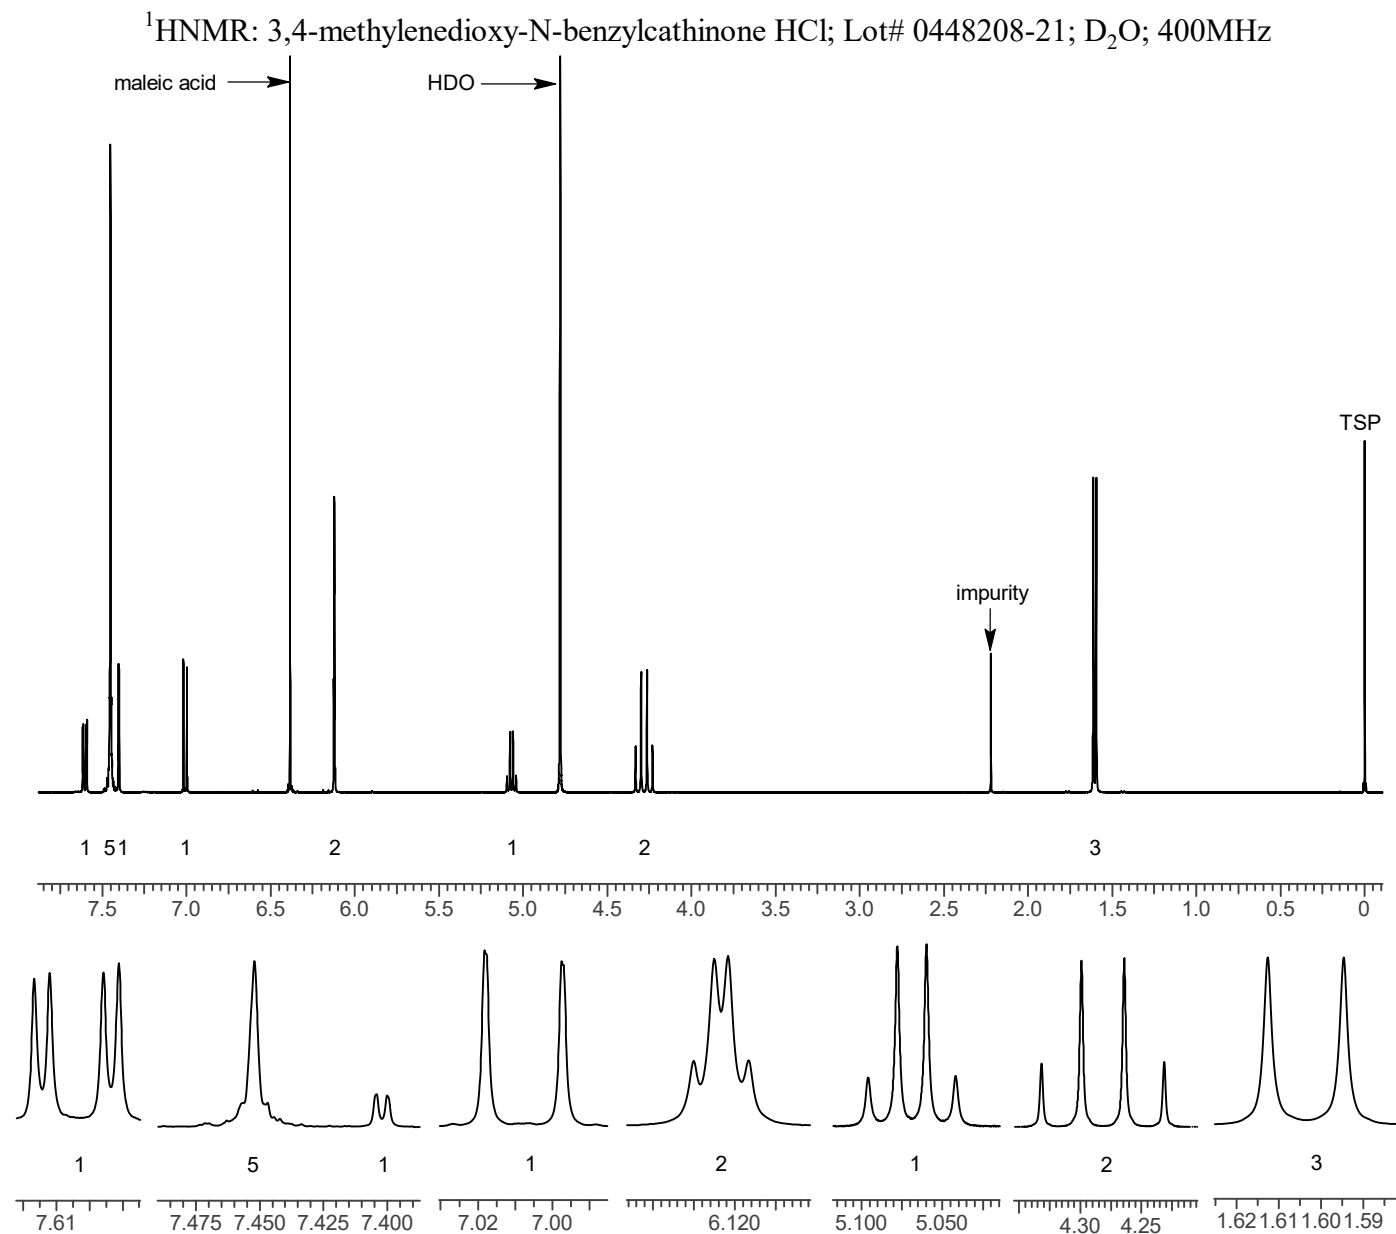



## 3,4-Methylenedioxy-N-benzylcathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



### 3.2 GAS CHROMATOGRAPHY/MASS SPECTROMETRY

**Sample Preparation:** Dilute analyte ~4 mg/mL in CHCl<sub>3</sub>, base extracted

**Instrument:** Agilent gas chromatograph operated in split mode with MS detector

**Column:** HP-5 MS (or equivalent); 30m x 0.25 mm x 0.25 μm

**Carrier Gas:** Helium at 1.5 mL/min

**Temperatures:** Injector: 280°C                      MSD transfer line: 280°C

MS Source: 230°C                      MS Quad: 150°C

Oven program:

1) 100°C initial temperature for 1.0 min

2) Ramp to 280°C at 12 °C/min

3) Hold final temperature for 9.0 min



**Injection Parameters:** Split Ratio = 25:1, 1 μL injected

**MS Parameters:** Mass scan range: 30-550 amu                      Threshold: 250

Tune file: stune.u                      Acquisition mode: scan

**Retention Time:** 14.03 min

EI Mass Spectrum: 3,4-methylenedioxy-N-benzylcathinone HCl; Lot# 0448208-21

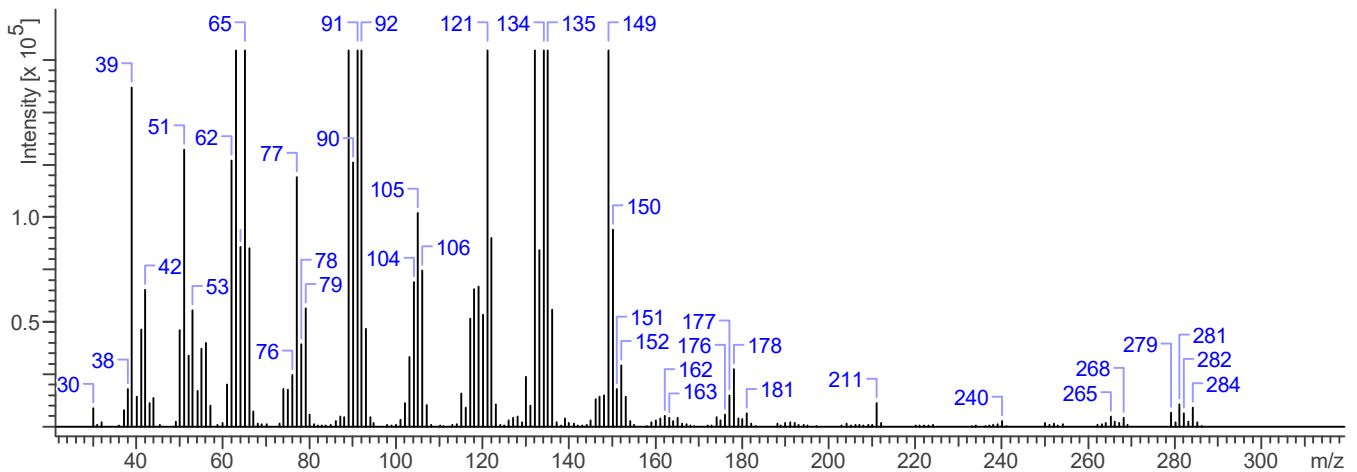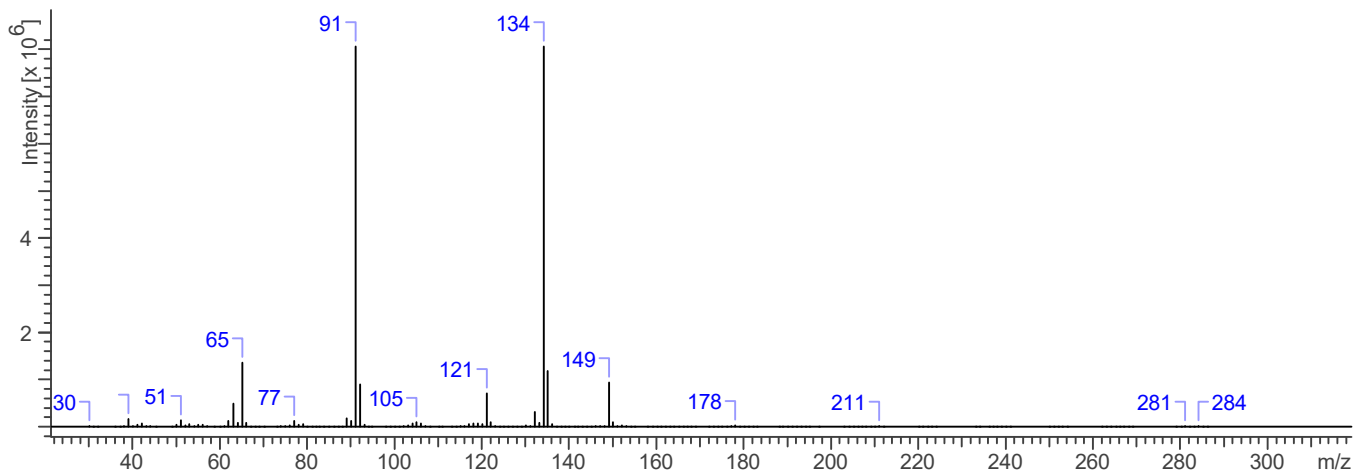



# 3,4-Methylenedioxy-N-benzylcathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



## 3.3 INFRARED SPECTROSCOPY (FTIR)

**Instrument:** FTIR with diamond ATR attachment (1 bounce)

**Scan Parameters:**  
Number of scans: 32  
Number of background scans: 32  
Resolution: 4 cm<sup>-1</sup>  
Sample gain: 1  
Aperture: 150

FTIR ATR (Diamond 1 Bounce): 3,4-methylenedioxy-N-benzylcathinone HCl; Lot# 0448208-21

