




## Cyclopropyl Fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

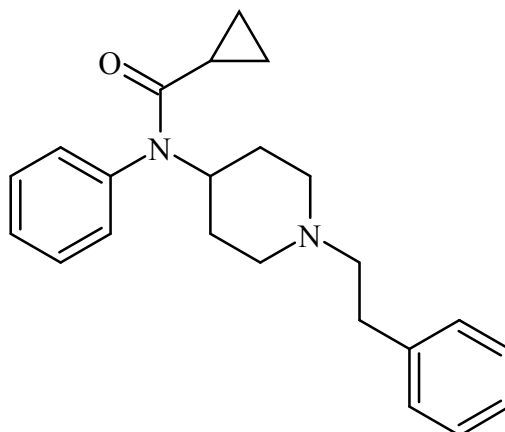

### 1. GENERAL INFORMATION

<b>IUPAC Name:</b>	N-(1-phenethylpiperidin-4-yl)-N-phenylcyclopropanecarboxamide
<b>CAS#:</b>	N/A
<b>Synonyms:</b>	N-phenyl-N-[1-(2-phenylethyl)piperidin-4-yl]cyclopropanecarboxamide
<b>Source:</b>	DEA Reference Material Collection
<b>Appearance:</b>	Off-White powder
<b>UV<sub>max</sub>(nm):</b>	Not Determined

### 2. CHEMICAL AND PHYSICAL DATA

#### 2.1 CHEMICAL DATA

Form	Chemical Formula	Molecular Weight	Melting Point (°C)
Base	C <sub>23</sub> H <sub>28</sub> N <sub>2</sub> O	348.48	Not Determined
HCl	C <sub>23</sub> H <sub>28</sub> N <sub>2</sub> O HCl	384.94	Not Determined



# Cyclopropyl Fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




## 3. QUALITATIVE DATA

### 3.1 NUCLEAR MAGNETIC RESONANCE

**Sample Preparation:** Dilute analyte to ~4 mg/mL in CD<sub>3</sub>OD containing TMS for 0 ppm reference and dimethylfumarate as quantitative internal standard.

**Instrument:** 400 MHz NMR spectrometer  
**Parameters:** Spectral width: at least containing -3 ppm through 13 ppm  
Pulse angle: 90°  
Delay between pulses: 45 seconds

<sup>1</sup>HNMR: Cyclopropyl fentanyl HCl, Lot 0505024-23, CD<sub>3</sub>OD, 400MHz  
Dimethylfumarate

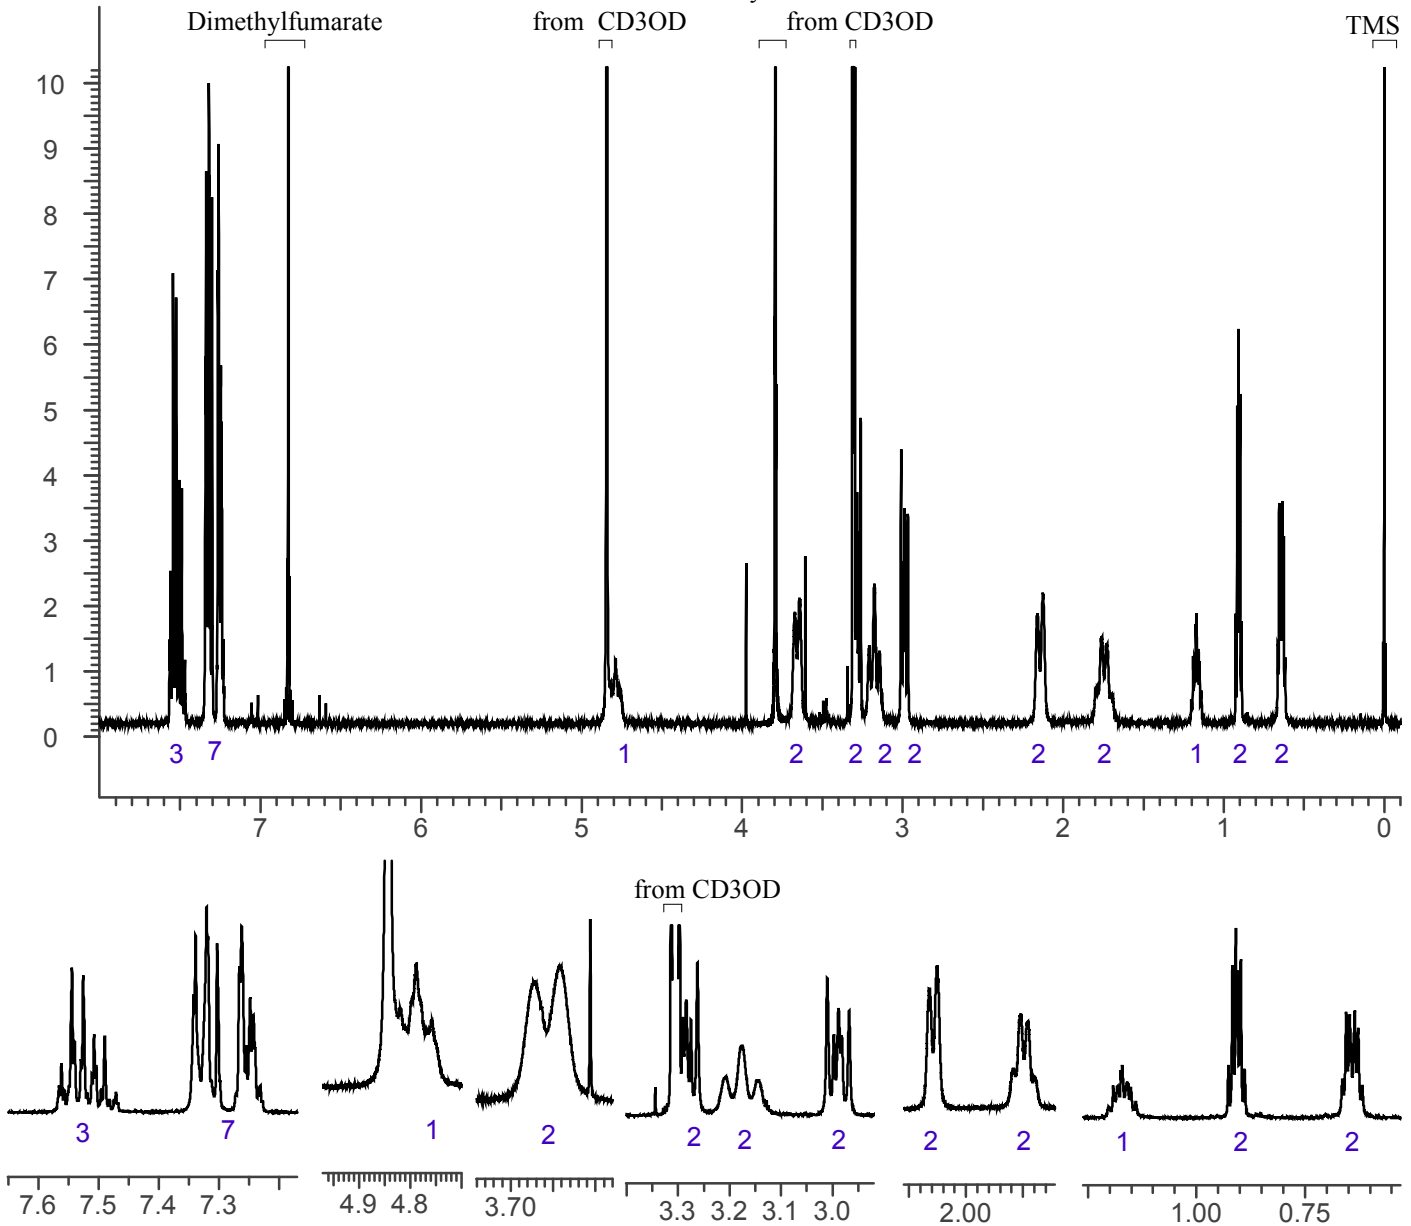



# Cyclopropyl Fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



## 3.2 GAS CHROMATOGRAPHY/MASS SPECTROMETRY


**Sample Preparation:** Dilute analyte ~4 mg/mL in Methanol.

**Instrument:** Agilent gas chromatograph operated in split mode with MS detector  
**Column:** HP-5 MS (or equivalent); 30m x 0.25 mm x 0.25  $\mu$ m  
**Carrier Gas:** Helium at 1.5 mL/min  
**Temperatures:** Injector: 280°C  
MSD transfer line: 280°C  
MS Source: 230°C  
MS Quad: 150°C  
Oven program:  
1) 100°C initial temperature for 1.0 min  
2) Ramp to 280°C at 12 °C/min  
3) Hold final temperature for 9.0 min

**Injection Parameters:** Split Ratio = 25:1, 1  $\mu$ L injected  
**MS Parameters:** Mass scan range: 30-550 amu  
Threshold: 100  
Tune file: stune.u  
Acquisition mode: scan

**Retention Time:** 17.974 min

EI Mass Spectrum: Cyclopropyl Fentanyl HCl; Lot # 0505024-23

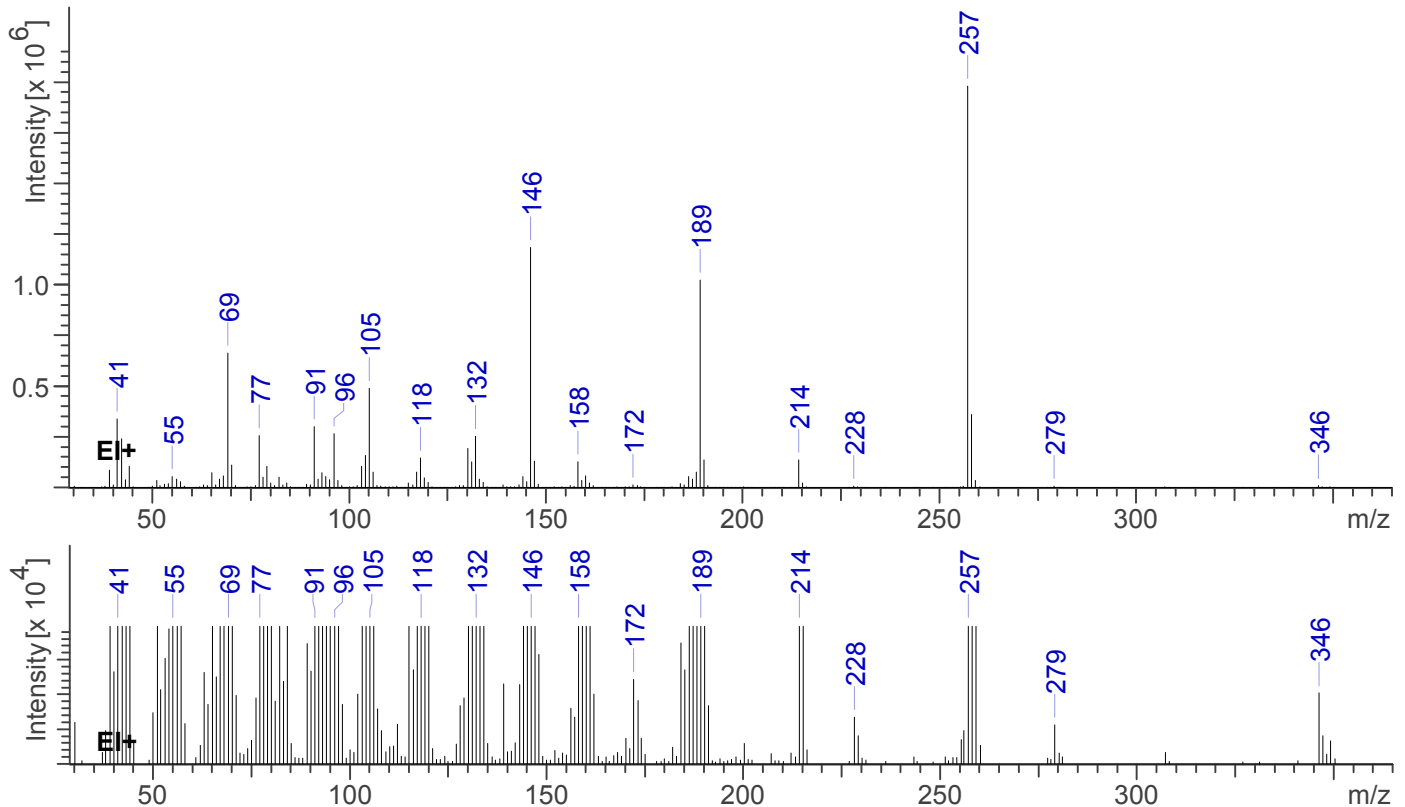



# Cyclopropyl Fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.





## 3.3 INFRARED SPECTROSCOPY (FTIR)

**Instrument:** FTIR with diamond ATR attachment (3 bounce)

**Scan Parameters:**  
Number of scans: 16  
Number of background scans: 16  
Resolution: 4 cm<sup>-1</sup>  
Sample gain: 8  
Aperture: 150

FTIR ATR (Diamond, 3 Bounce): Cyclopropyl Fentanyl HCl; Lot# 0505024-23

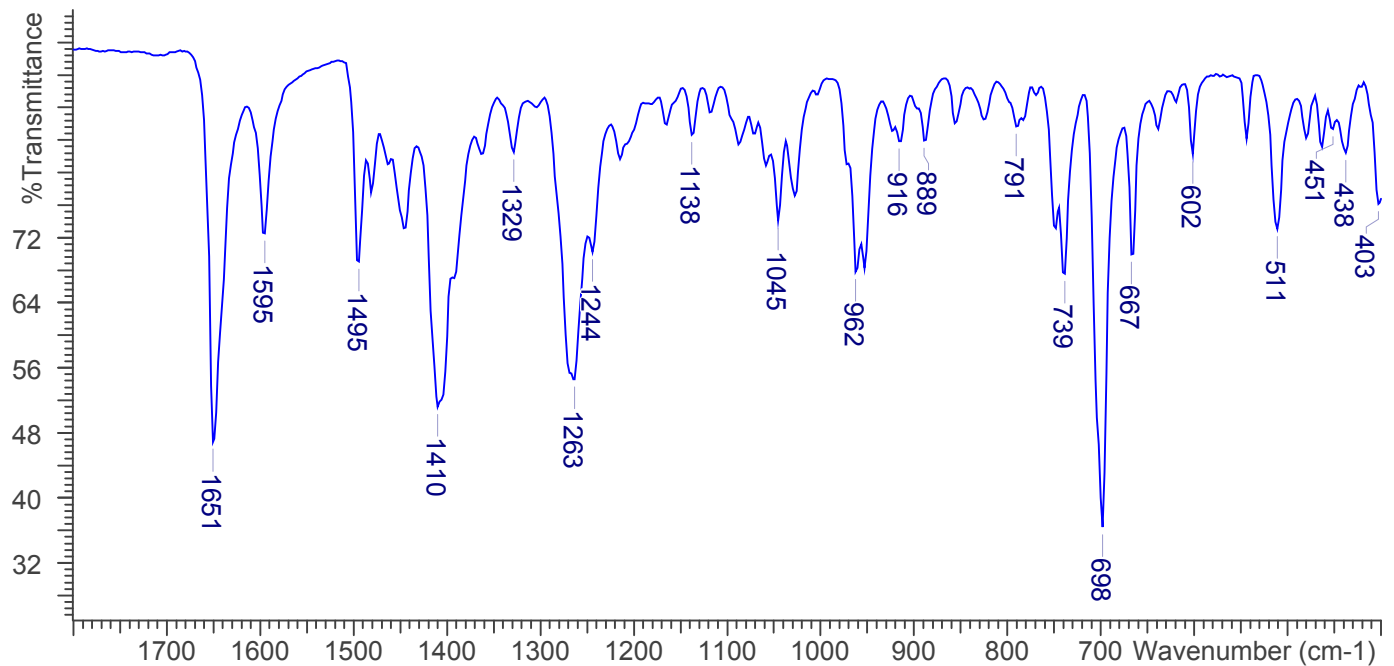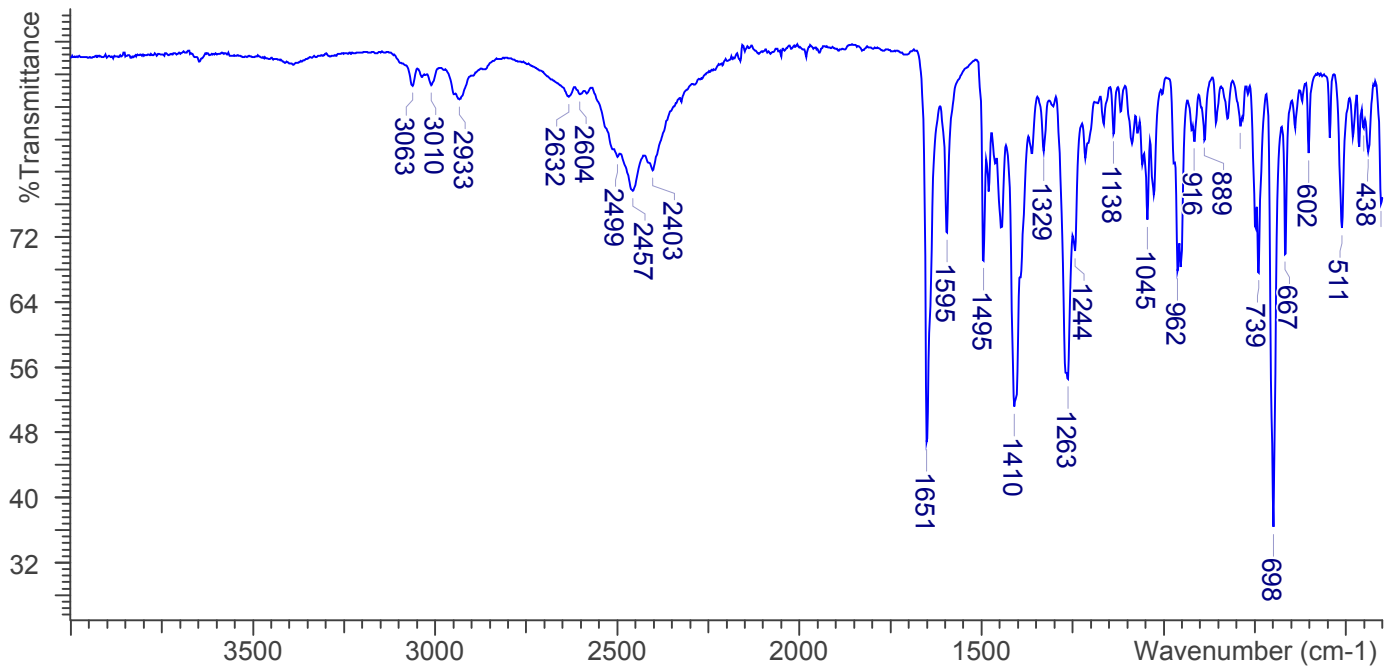



## Cyclopropyl Fentanyl

*The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.*



### **4. ADDITIONAL RESOURCES**

*No Literature available as of 8/2017*