




DiPT

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

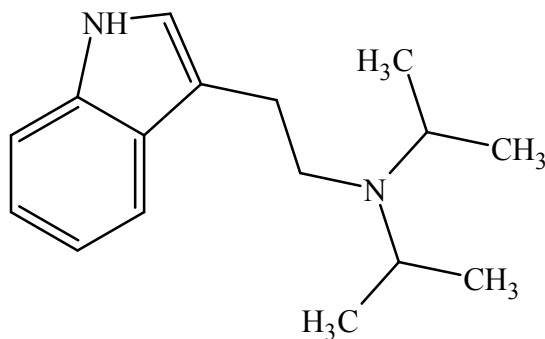

1. GENERAL INFORMATION

IUPAC Name:	N-[2-(1H-indol-3-yl)ethyl]-N-(propan-2-yl)propan-2-amine
CAS#:	14780-24-6 (base)
Synonyms:	N,N-diisopropyltryptamine, N,N-bis(1-methylethyl)-1H-indole-3-ethanamine
Source:	DEA Reference Material Collection
Appearance:	White Powder (HCl)
UV_{max} (nm):	Not Determined

2. CHEMICAL AND PHYSICAL DATA

2.1 CHEMICAL DATA

Form	Chemical Formula	Molecular Weight	Melting Point (°C)
Base	C ₁₆ H ₂₄ N ₂	244	Not Determined
HCl	C ₁₆ H ₂₄ N ₂ · HCl	280	197.0



DiPT

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




3. QUALITATIVE DATA

3.1 NUCLEAR MAGNETIC RESONANCE

Sample Preparation: Dilute analyte to ~20 mg/mL in deuterium oxide (D₂O) containing TSP for 0 ppm reference and maleic acid as quantitative internal standard.

Instrument: 400 MHz NMR spectrometer
Parameters: Spectral width: at least containing -3 ppm through 13 ppm
Pulse angle: 90°
Delay between pulses: 45 seconds

¹H NMR: DiPT HCl; Lot H-0404; D₂O; 400 MHz

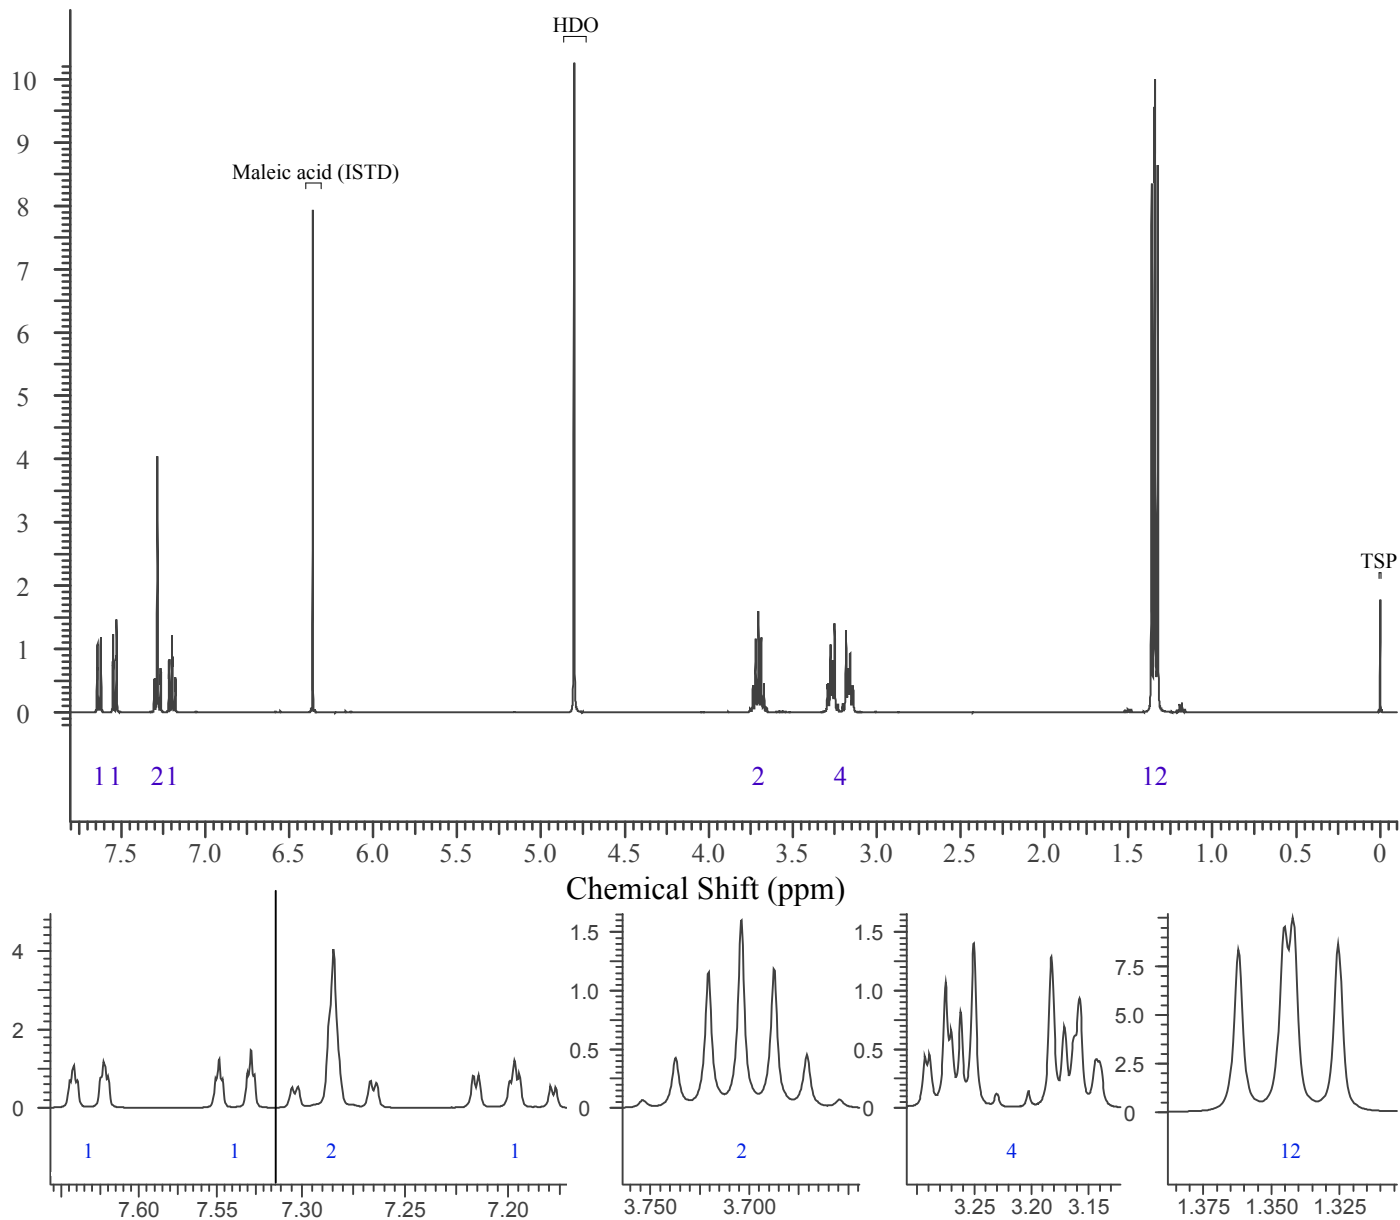



DiPT

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



3.2 Gas Chromatography/Mass Spectrometry

Sample Preparation: Dilute analyte ~ 4 mg/mL base extracted into chloroform

Instrument: Agilent gas chromatograph operated in split mode with MS detector

Column: DB-1 MS (or equivalent); 30m x 0.25 mm x 0.25 μ m

Carrier Gas: Helium at 1 mL/min

Temperatures: Injector: 280°C
MSD transfer line: 280°C

MS Source: 230°C

MS Quad: 150°C

Oven program:

1) 90°C initial temperature for 2.0 min

2) Ramp to 300°C at 14 °C/min

3) Hold final temperature for 10.0 min

Injection Parameters: Split Ratio = 25:1, 1 μ L injected

MS Parameters: Mass scan range: 34-550 amu



Threshold: 100

Tune file: stune.u

Acquisition mode: scan

Retention Time: 12.838 min

EI Mass Spectrum: DiPT HCl; Lot H-0404

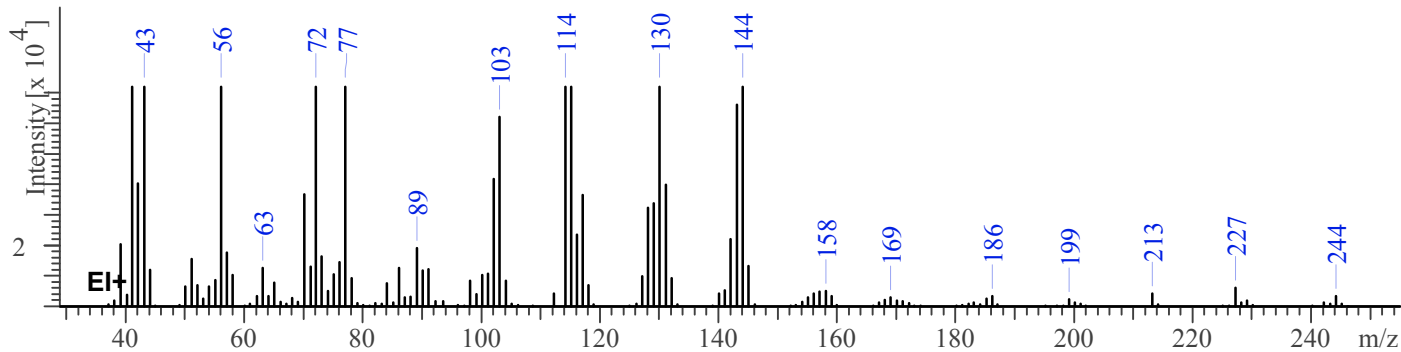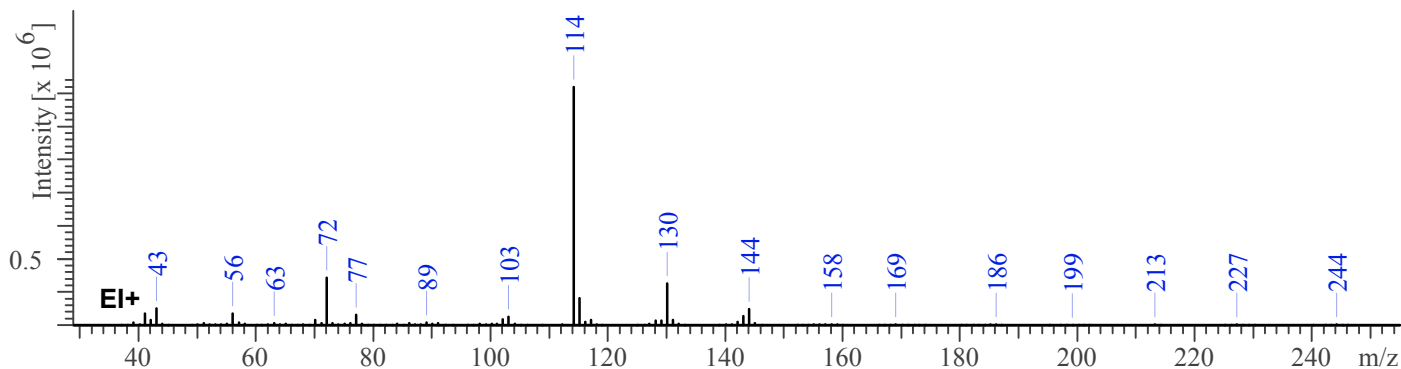



DiPT

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.





3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR with diamond ATR attachment (3 bounce)

Scan Parameters:
Number of scans: 32
Number of background scans: 32
Resolution: 4 cm⁻¹
Sample gain: 8
Aperture: 150

FTIR ATR (Diamond, 3 Bounce): DiPT HCl; Lot H-0404

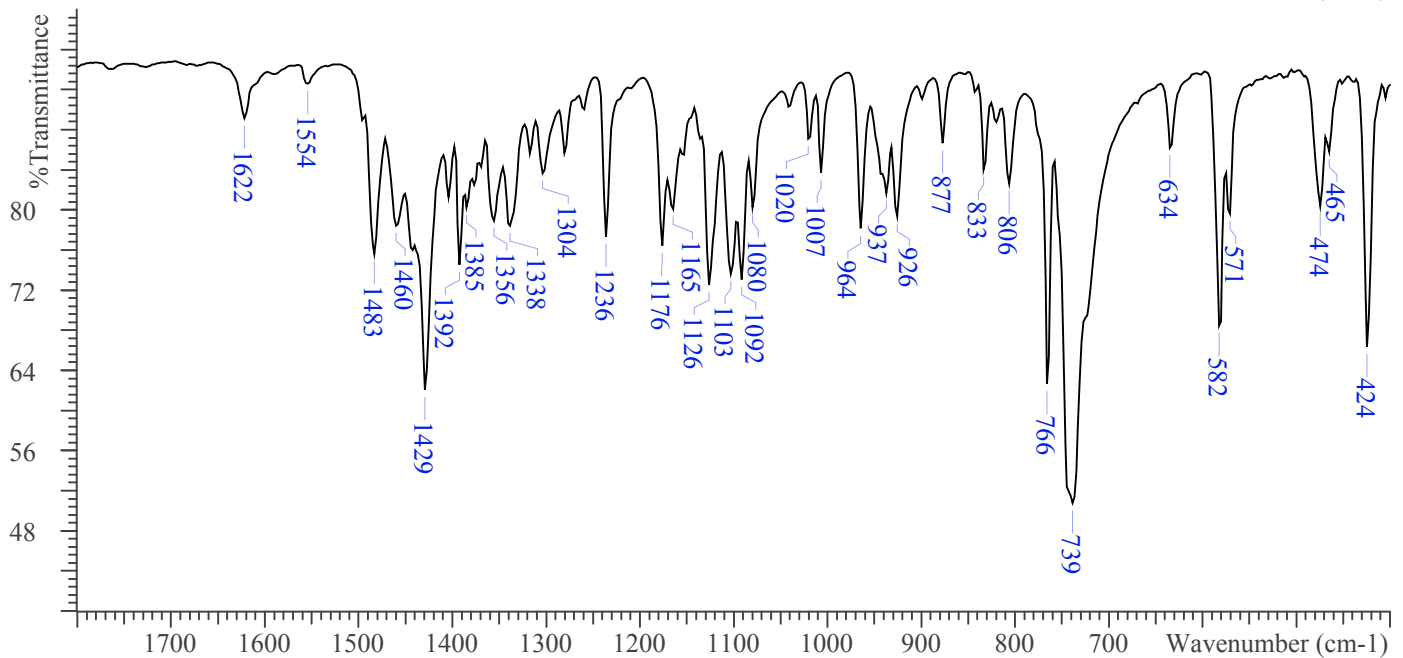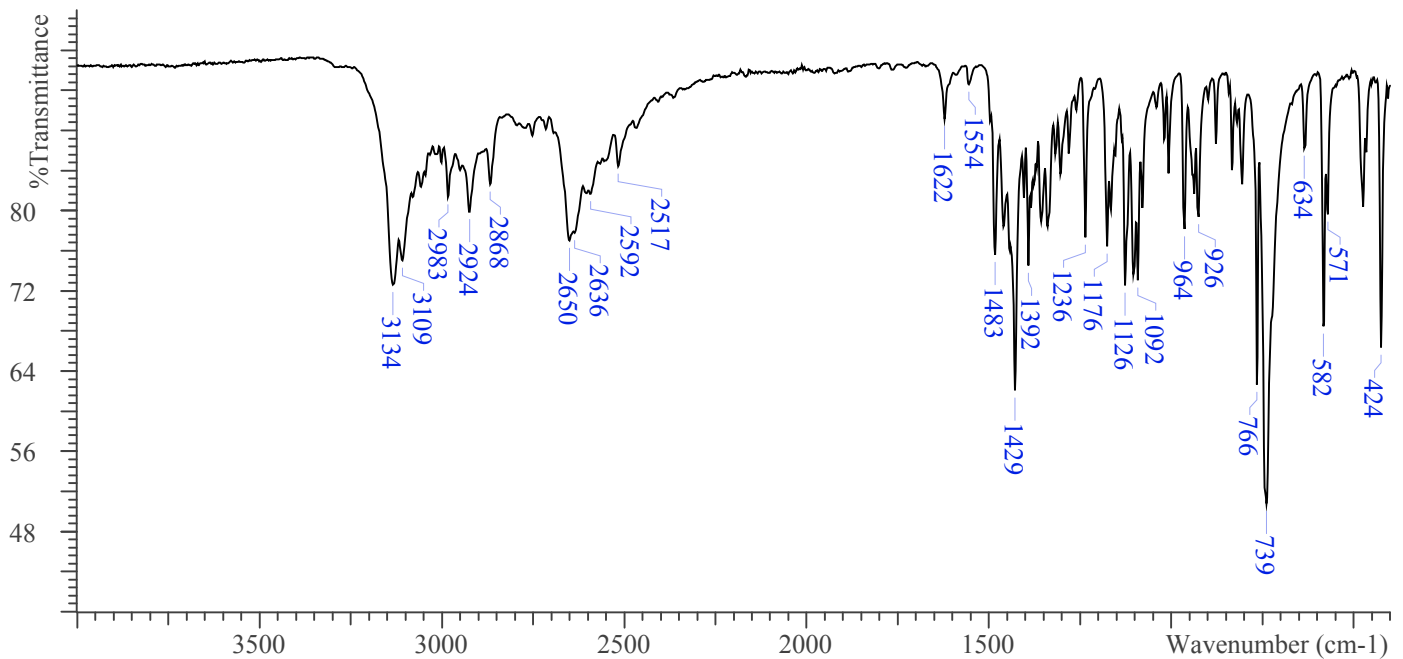



DiPT

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



4. **ADDITIONAL RESOURCES**

[Wikipedia](#)