









U-49900

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.





### 3.3 INFRARED SPECTROSCOPY (FTIR)

**Instrument:** FTIR (Smart Golden Gate ATR Accessory)

**Scan Parameters:**  
Number of scans: 32  
Number of background scans: 32  
Resolution: 4 cm<sup>-1</sup>  
Sample gain: 8  
Aperture: 150

FTIR ATR (Diamond1 Bounce): U-49900; lot# 0497502-22

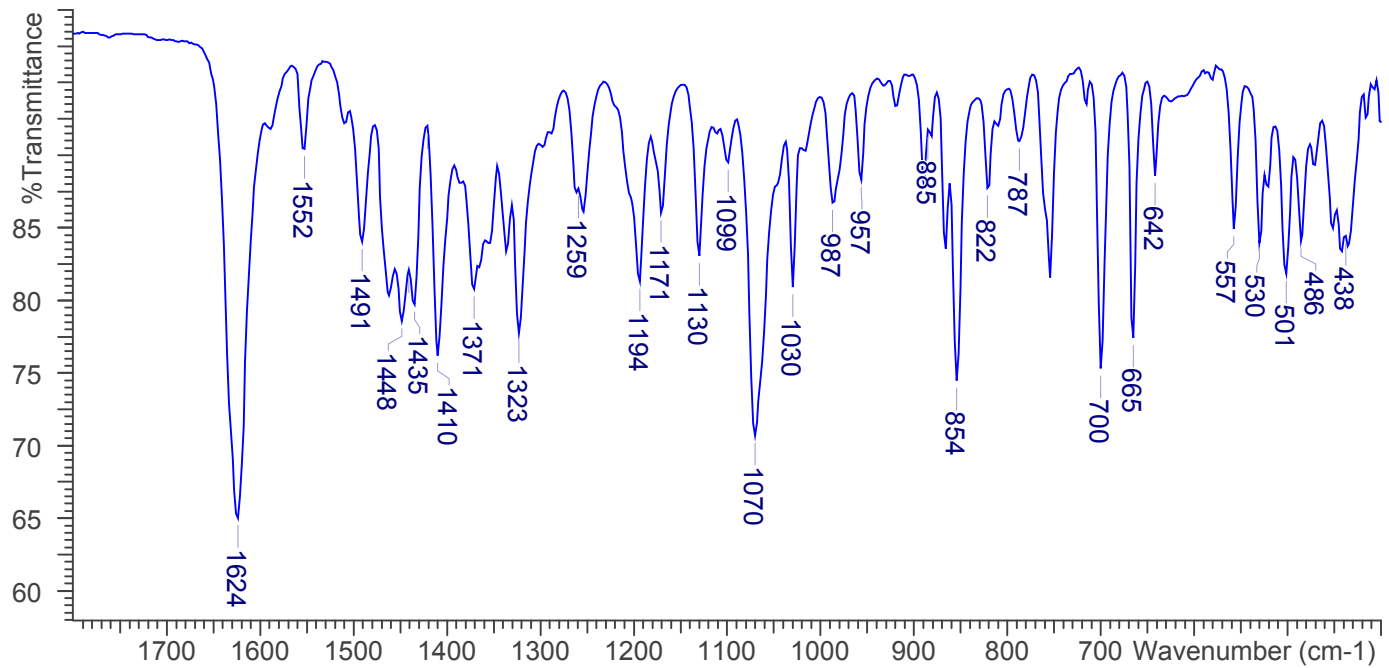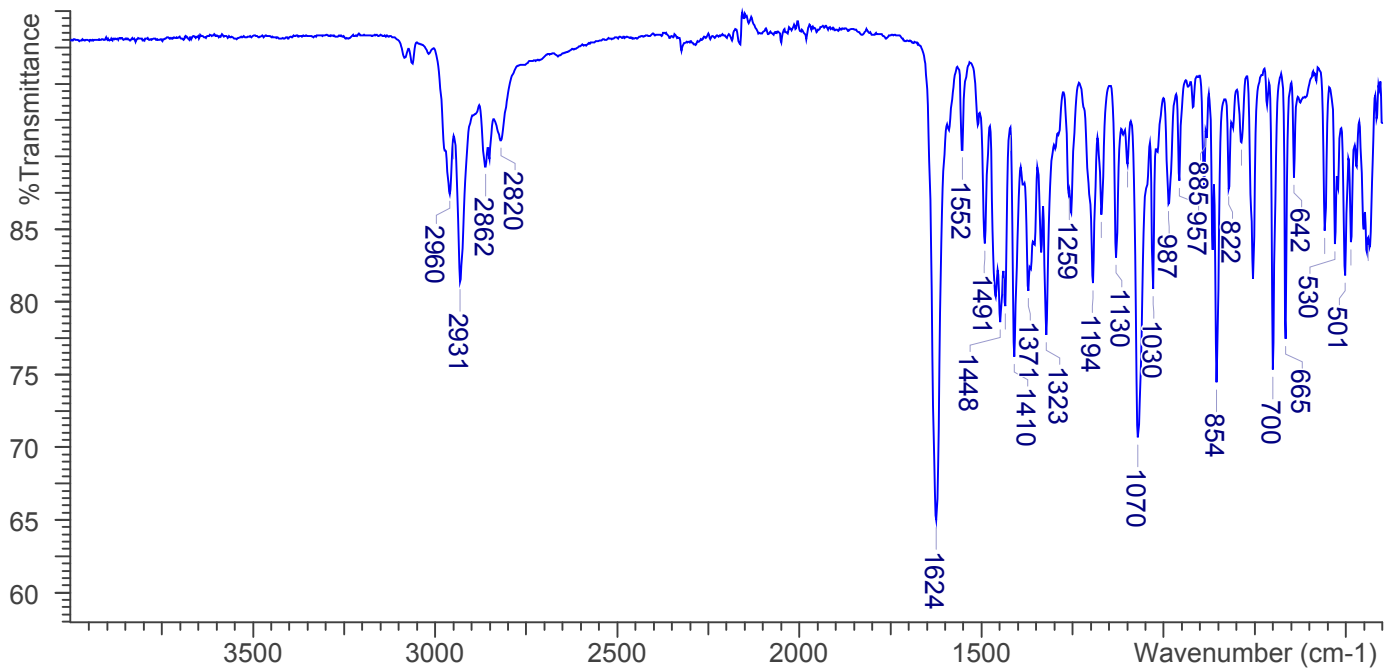



**U-49900**



*The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.*

#### **4. ADDITIONAL RESOURCES**

*No available literature as of 11/30/17*