




meta-Fluoroisobutyryl fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

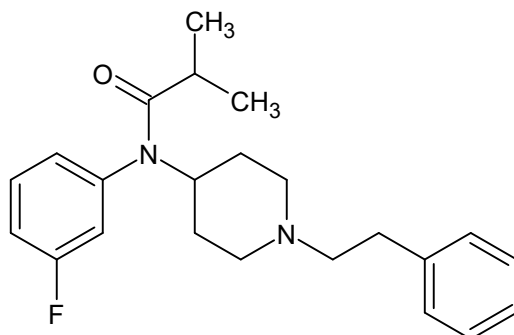

1. GENERAL INFORMATION

IUPAC Name:	<i>N</i> -(3-fluorophenyl)- <i>N</i> -(1-phenethylpiperidin-4-yl)isobutyramide
CAS#:	N/A
Synonyms:	3-FIBF, m-FIBF, 3-fluoroisobutyryl fentanyl, m-fluoroisobutyryl fentanyl, <i>N</i> -(3-fluorophenyl)-2-methyl- <i>N</i> -[1-(2-phenylethyl)piperidin-4-yl]propanamide
Source:	DEA Reference Material Collection
Appearance:	White powder
UV_{max}(nm):	Not determined

2. CHEMICAL AND PHYSICAL DATA

2.1 CHEMICAL DATA

Form	Chemical Formula	Molecular Weight	Melting Point (°C)
Base	C ₂₃ H ₂₉ FN ₂ O	368.49	Not Determined
HCl	C ₂₃ H ₂₉ FN ₂ O HCl	404.95	Not Determined



meta-Fluoroisobutyryl fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




3. QUALITATIVE DATA

3.1 NUCLEAR MAGNETIC RESONANCE

Sample Preparation: Dilute analyte to ~12 mg/mL in methanol- d_4 containing TMS for 0 ppm reference and 1,4-BTMSB- d_4 as quantitative internal standard.

Instrument: 400 MHz NMR spectrometer
Parameters: Spectral width: at least containing -3 ppm through 13 ppm
Pulse angle: 90°
Delay between pulses: 45 seconds

^1H NMR: *meta*-fluoroisobutyryl fentanyl HCl; Lot# 0538870-1; methanol- d_4 ; 400MHz

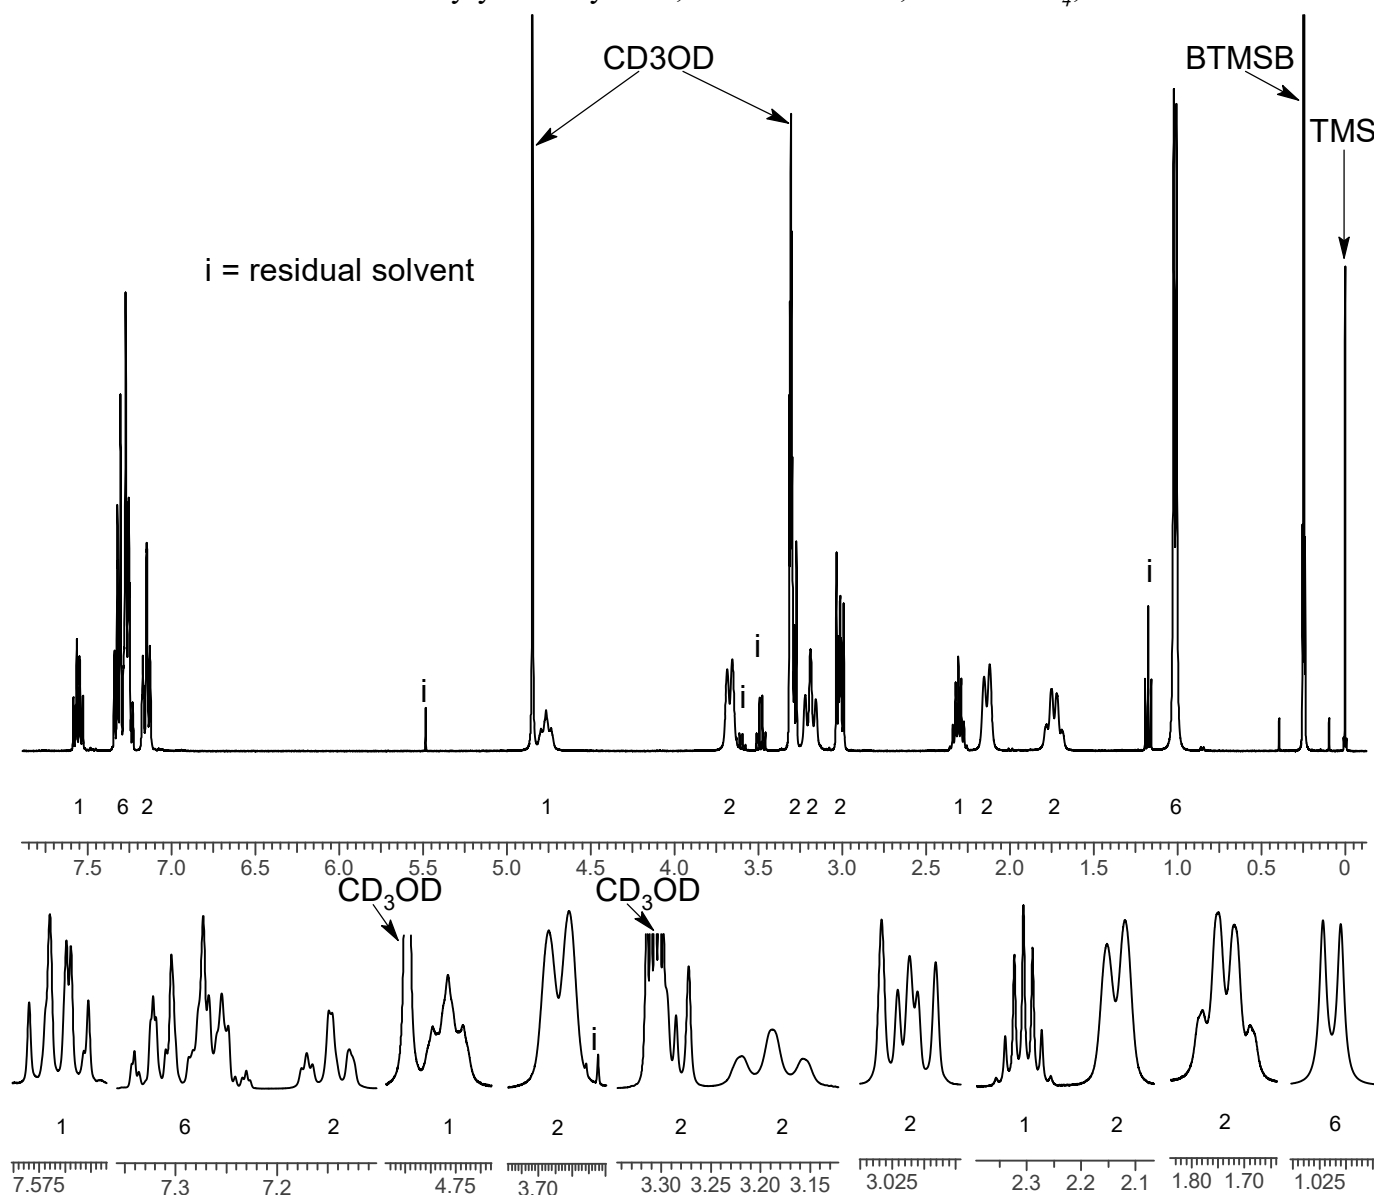



meta-Fluoroisobutyryl fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



3.2 GAS CHROMATOGRAPHY/MASS SPECTROMETRY

Sample Preparation: Dilute analyte ~5 mg/mL in MeOH

Instrument: Agilent gas chromatograph operated in split mode with MS detector

Column: HP-5 MS (or equivalent); 30m x 0.25 mm x 0.25 μ m

Carrier Gas: Helium at 1.5 mL/min

Temperatures: Injector: 280°C MSD transfer line: 280°C

MS Source: 230°C MS Quad: 150°C

Oven program:

1) 100°C initial temperature for 1.0 min

2) Ramp to 280°C at 12 °C/min

3) Hold final temperature for 9.0 min



Injection Parameters: Split Ratio = 25:1, 1 μ L injected

MS Parameters: Mass scan range: 30-550 amu Threshold: 150

Tune file: stune.u Acquisition mode: scan

Retention Time: 16.34 min

EI Mass Spectrum: *meta*-fluoroisobutyryl fentanyl HCl; Lot# 0538870-1

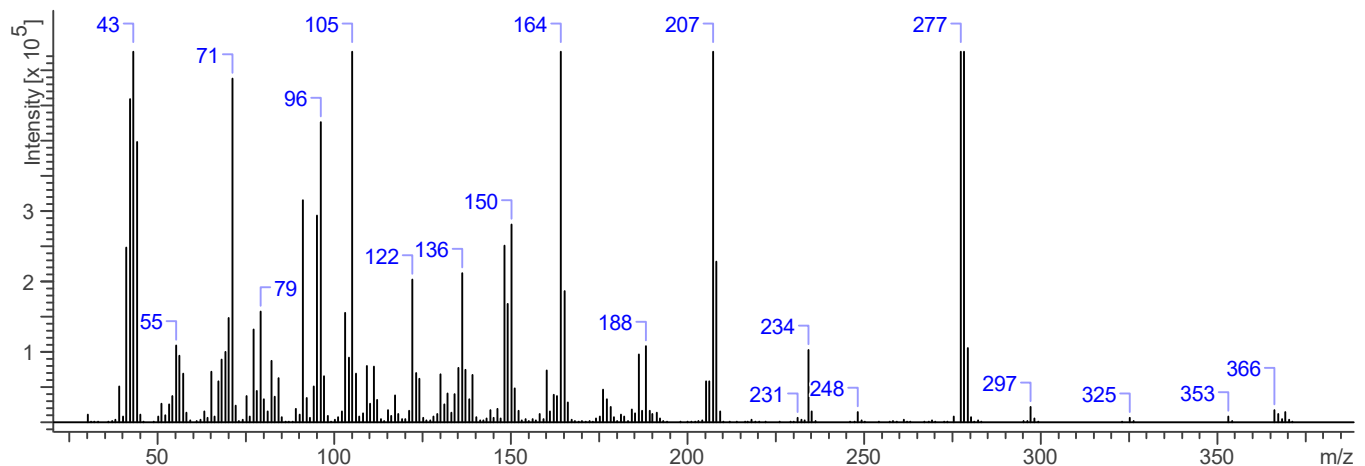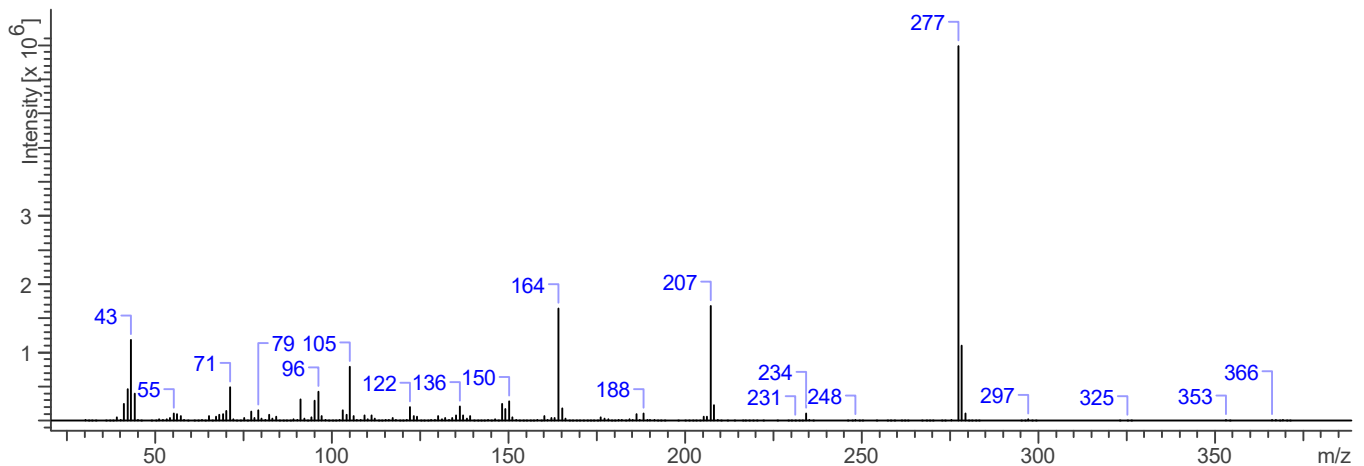



meta-Fluoroisobutyryl fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR with diamond ATR attachment (1 bounce)
Scan Parameters: Number of scans: 32
Number of background scans: 32
Resolution: 4 cm⁻¹
Sample gain: 1
Aperture: 150

FTIR ATR (Diamond 1 Bounce): meta-fluoroisobutyryl fentanyl HCl; Lot# 0538870-1

