



4-Fluoropentedrone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.





3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR with Golden Gate diamond ATR attachment (1 bounce)

Scan Parameters:
Number of scans: 16
Number of background scans: 16
Resolution: 4 cm⁻¹
Sample gain: 8
Aperture: 150

FTIR (Golden Gate with ATR, 1 Bounce): 4-Fluoropentedrone HCl; Lot 0464459-21

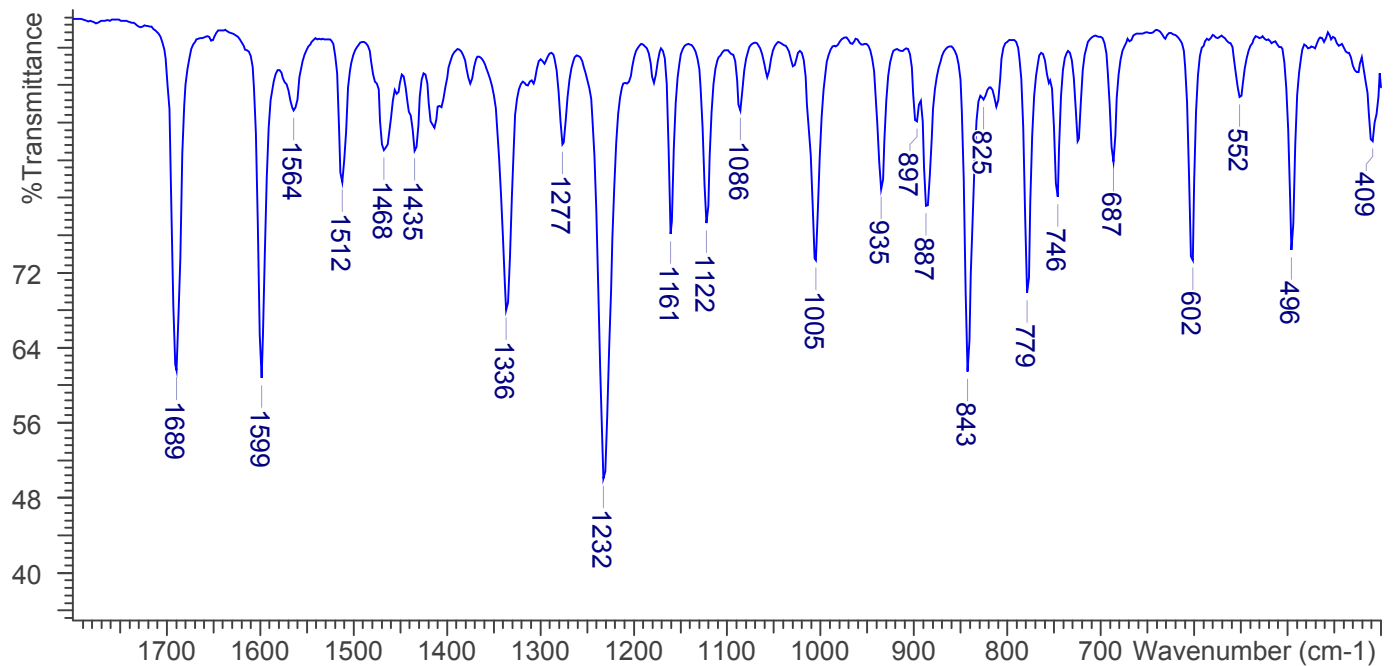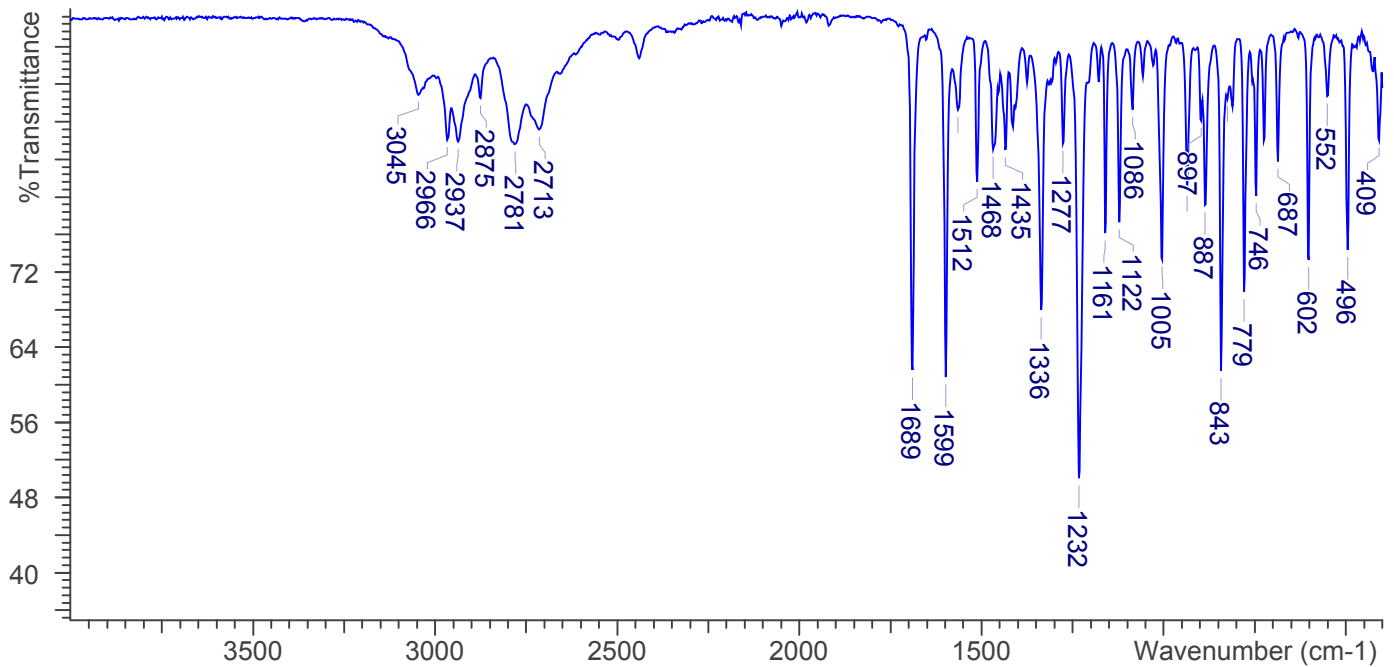



4-Fluoropentedrone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



4. ADDITIONAL RESOURCES

No Literature as of 08/2017