




para-Fluorofentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

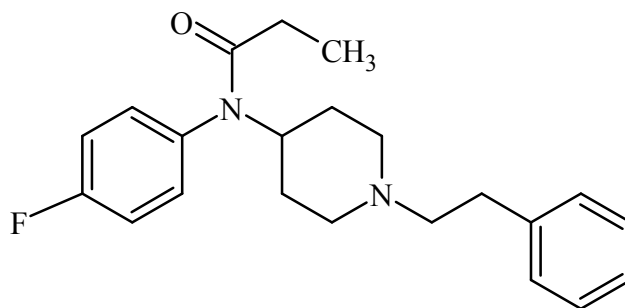

1. GENERAL INFORMATION

IUPAC Name:	N-(4-fluorophenyl)-N-[1-(2-phenylethyl)-4-piperidinyl]propionamide
CAS#:	NA
Synonyms:	NA
Source:	DEA Reference Material Collection
Appearance:	white powder
UV_{max}(nm):	NA

2. CHEMICAL AND PHYSICAL DATA

2.1 CHEMICAL DATA

Form	Chemical Formula	Molecular Weight	Melting Point (°C)
Base	C ₂₂ H ₂₇ FN ₂ O	354.54	NA
HCl	C ₂₂ H ₂₇ FN ₂ O · HCl	391.00	NA



para-Fluorofentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




3. QUALITATIVE DATA

3.1 NUCLEAR MAGNETIC RESONANCE

Sample Preparation: Dilute analyte to ~22 mg/mL in CD₃OD containing TMS for 0 ppm reference and 1,4-BTMSB-d₄ as quantitative internal standard.

Instrument: 400 MHz NMR spectrometer
Parameters: Spectral width: at least containing -3 ppm through 13 ppm
Pulse angle: 90°
Delay between pulses: 45 seconds

¹HNMR: para-Fluorofentanyl HCl; Lot# 8/17/81 aa

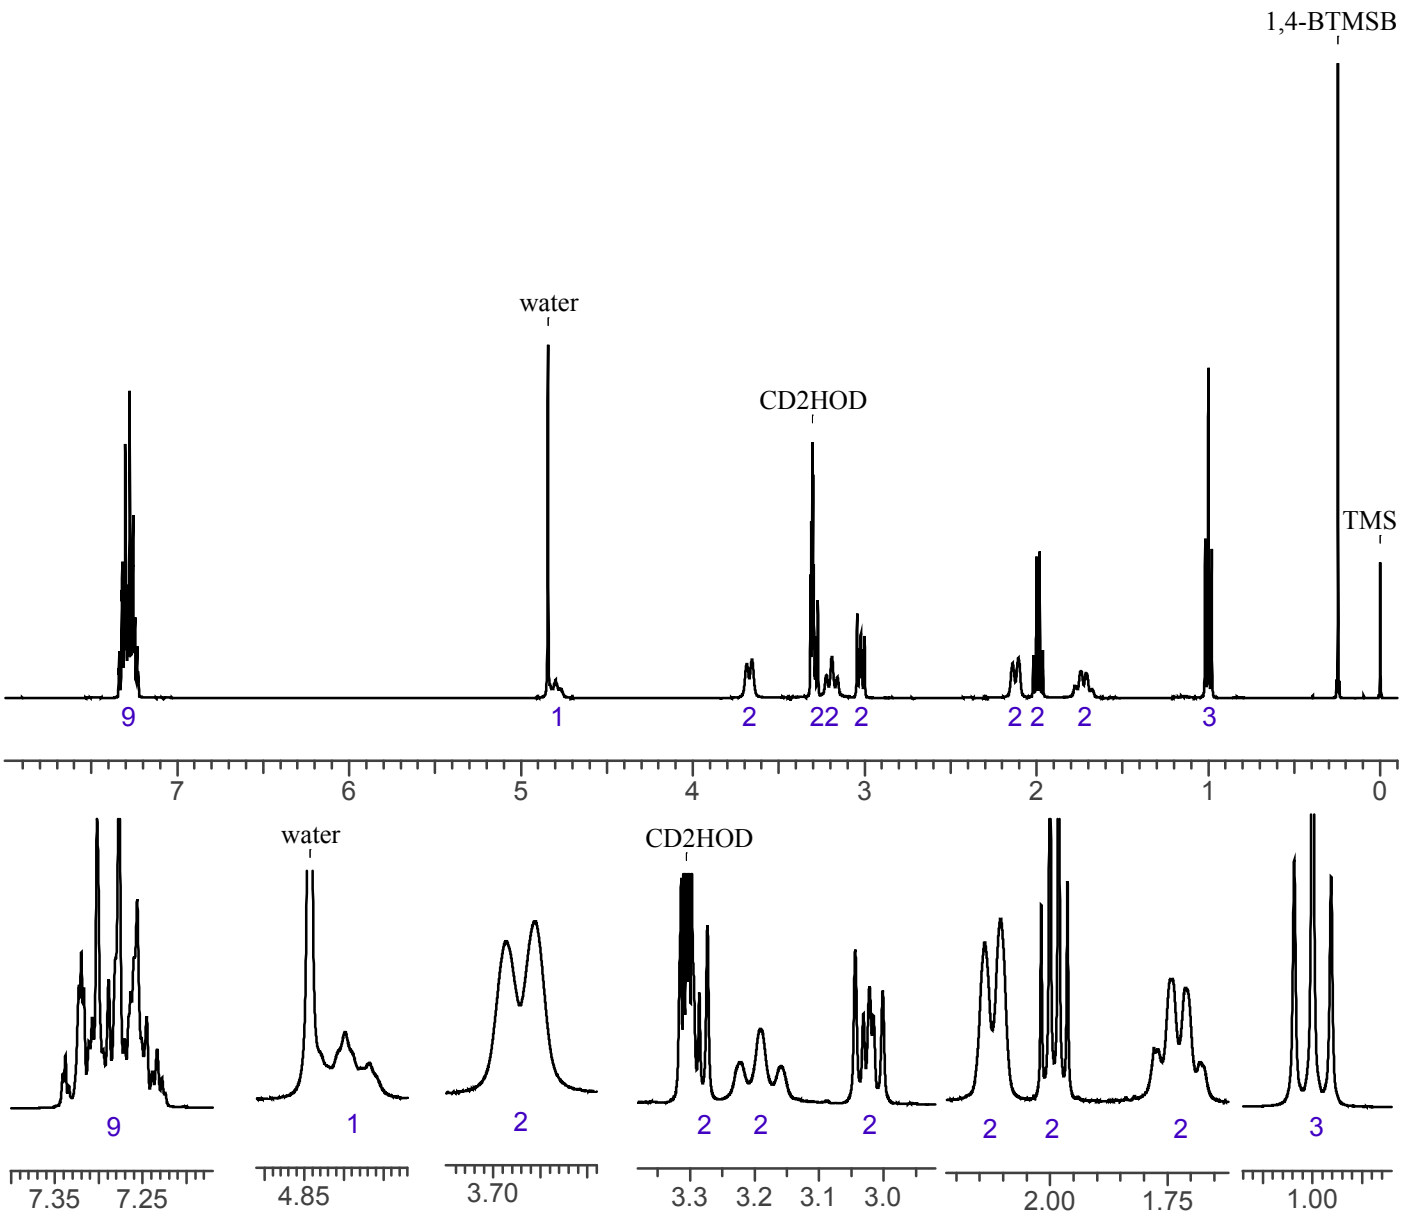



para-Fluorofentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



3.2 GAS CHROMATOGRAPHY/MASS SPECTROMETRY

Sample Preparation: Dilute analyte ~4 mg/mL into methanol.

Instrument: Agilent gas chromatograph operated in split mode with MS detector

Column: HP-5; 30m x 0.25 mm x 0.25 μ m

Carrier Gas: Helium at 1.5mL/min

Temperatures: Injector: 280°C

MSD transfer line: 280°C

MS Source: 230°C

MS Quad: 150°C

Oven program:

1) 100°C initial temperature for 1.0 min

2) Ramp to 280°C at 12 °C/min

3) Hold final temperature for 9.0 min

Injection Parameters: Split Ratio = 25:1, 1 μ L injected

MS Parameters: Mass scan range: 30-550 amu



Threshold: 100

Tune file: stune.u

Acquisition mode: scan

Retention Time: 16.261min

EI Mass Spectrum: para-Fluorofentanyl HCl; Lot# 8/17/81 aa

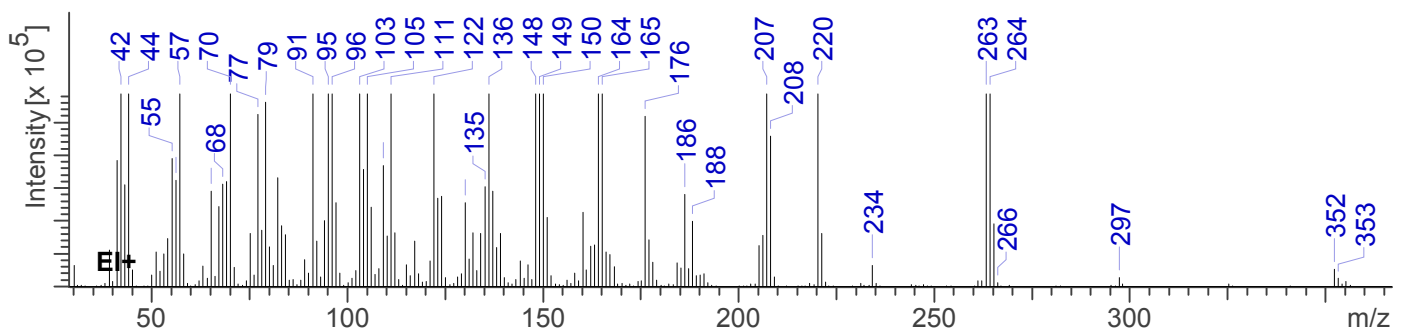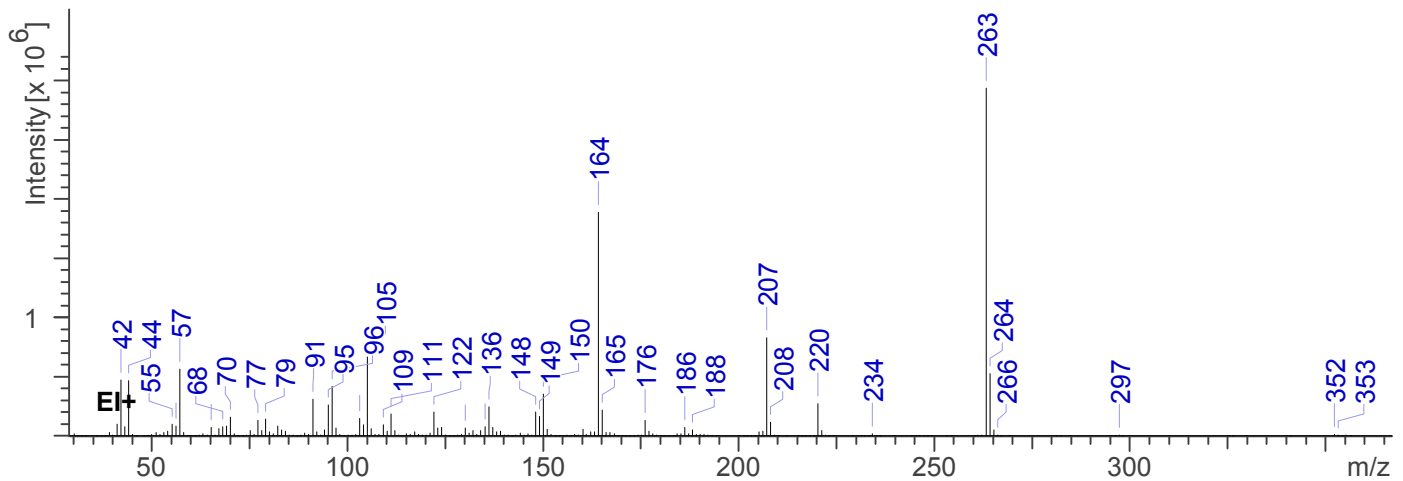



para-Fluorofentanyl





The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR with diamond ATR attachment (1 bounce)

Scan Parameters:
Number of scans: 32
Number of background scans: 32
Resolution: 4 cm⁻¹
Sample gain: 4
Aperture: 150

FTIR ATR (Diamond 1 Bounce): para-Fluorofentanyl HCl; Lot#8/17/81 aa

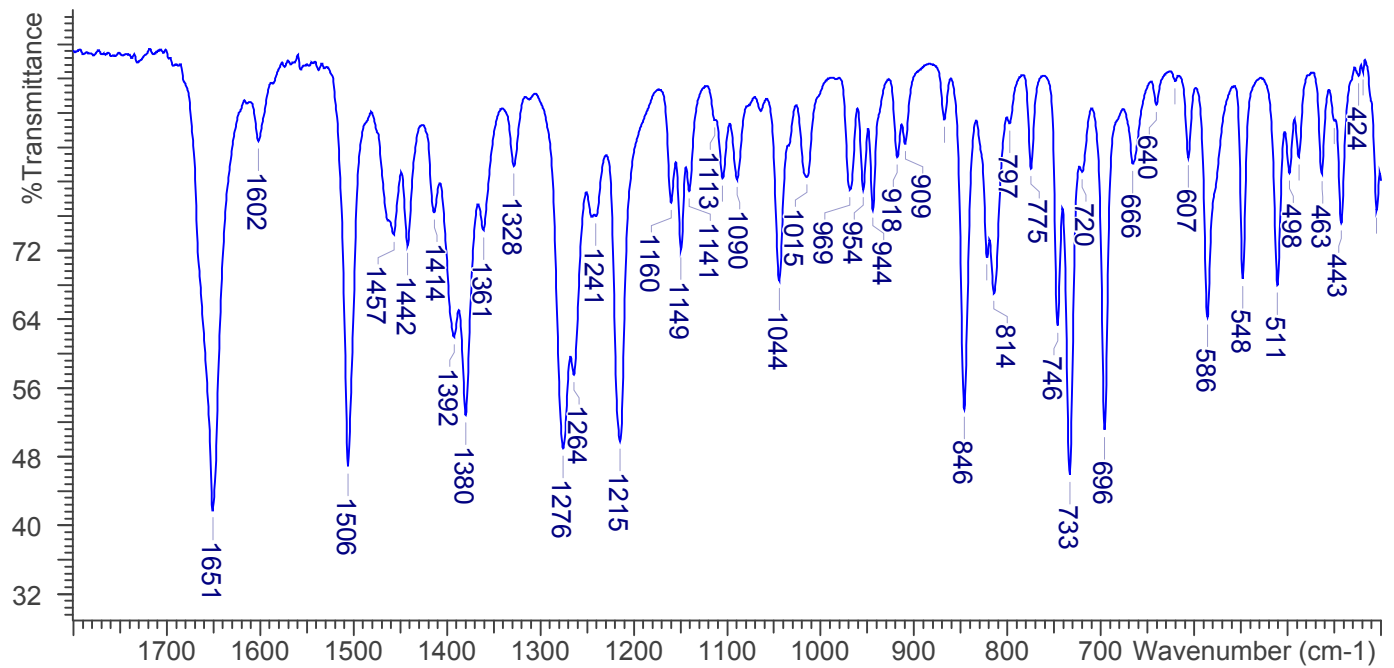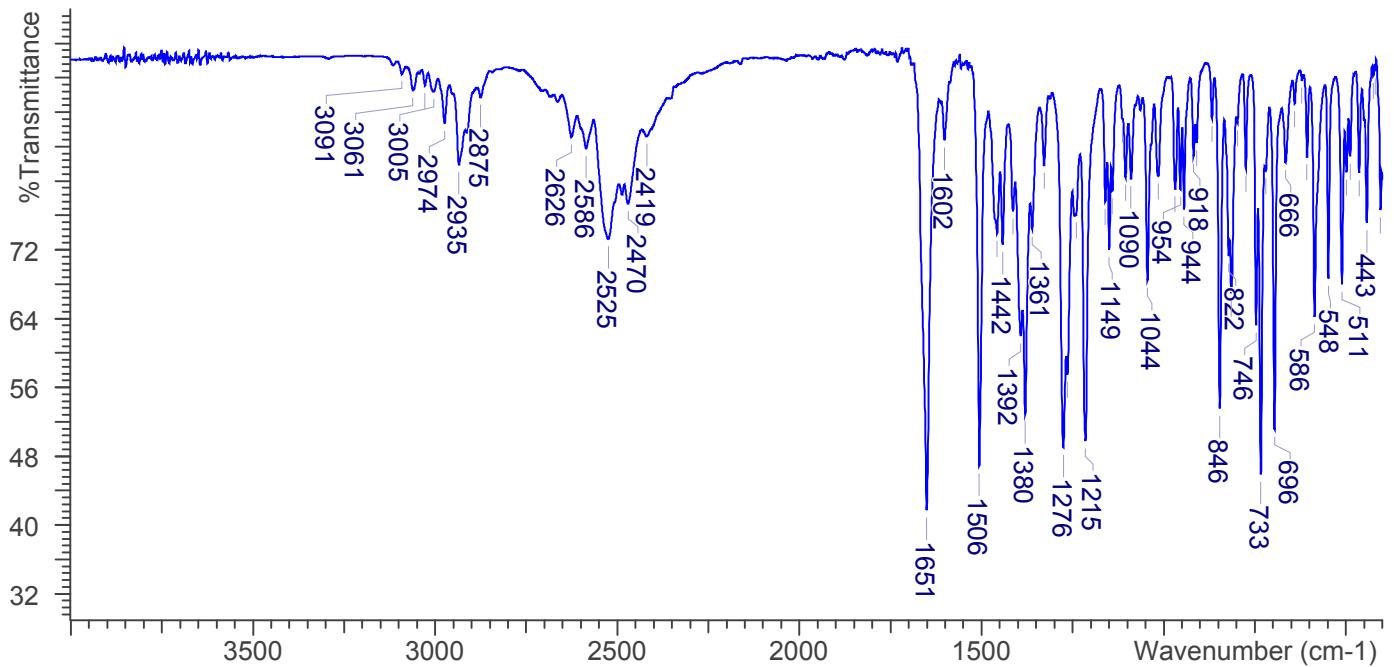



para-Fluorofentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.





3.4. GAS CHROMATOGRAPHY /INFRARED DETECTION:

Sample Preparation: Dilute analyte 1mg/ml in CHCl₃

Instrument: Gas Chromatograph in split mode with Infrared Detection
Column: HP-5; 30m x 0.32 mm id x 0.25 μm
Carrier Gas: Helium at 2.0mL/min
Temperature: Injector: 280°C Split ratio: 2:1, 2μl injection
65°C hold 0.5min., ramp to 310°C at 20°C/min., hold 5min.

IRD: Detector: Transfer line
Temp 280°C
Flow Cell Temp 280°C
Resolution 8 cm⁻¹

GC-IRD: para-Fluorofentanyl HCl; Lot# 8/17/81 aa

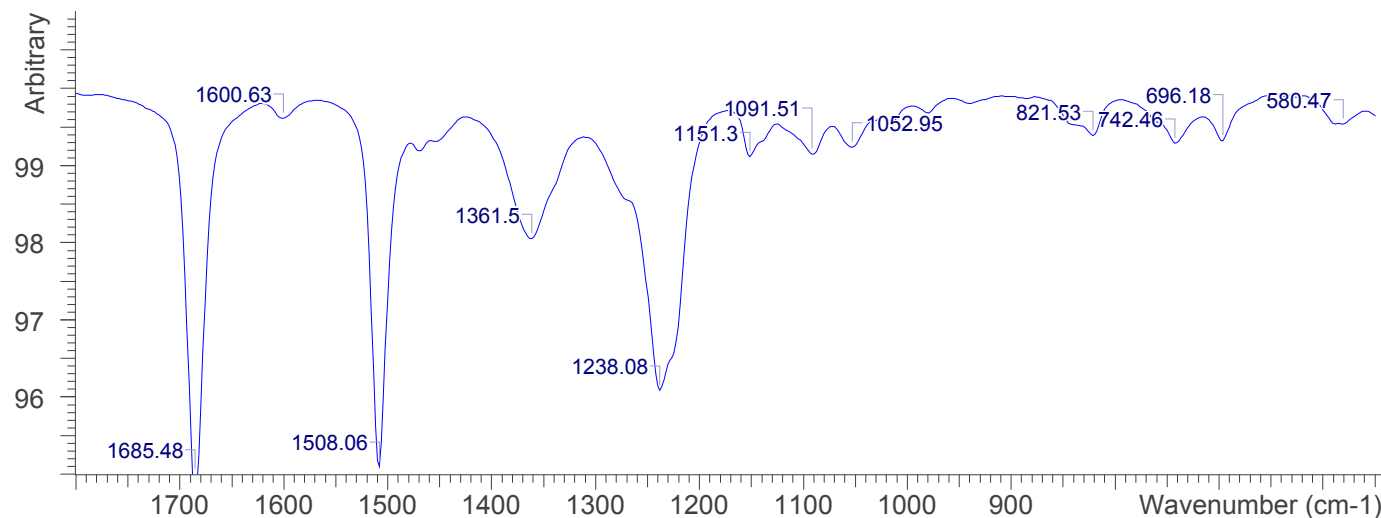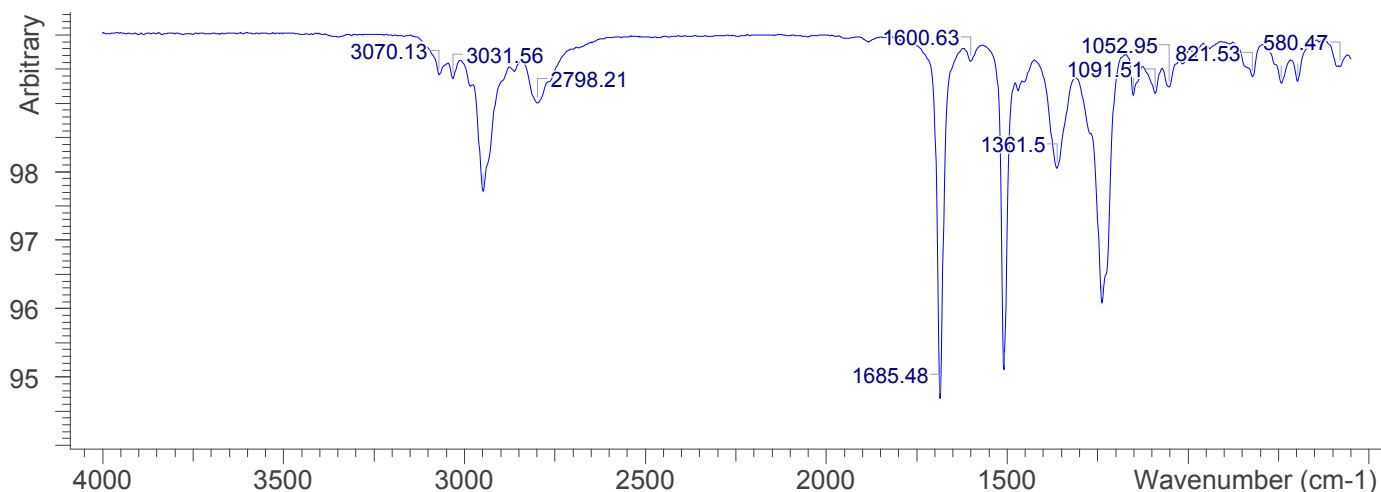



para-Fluorofentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



4. ADDITIONAL RESOURCES

No additional resources as of 07/02/2021